


Agilent B1505A Power Device Analyzer/Curve Tracer

Data Sheet

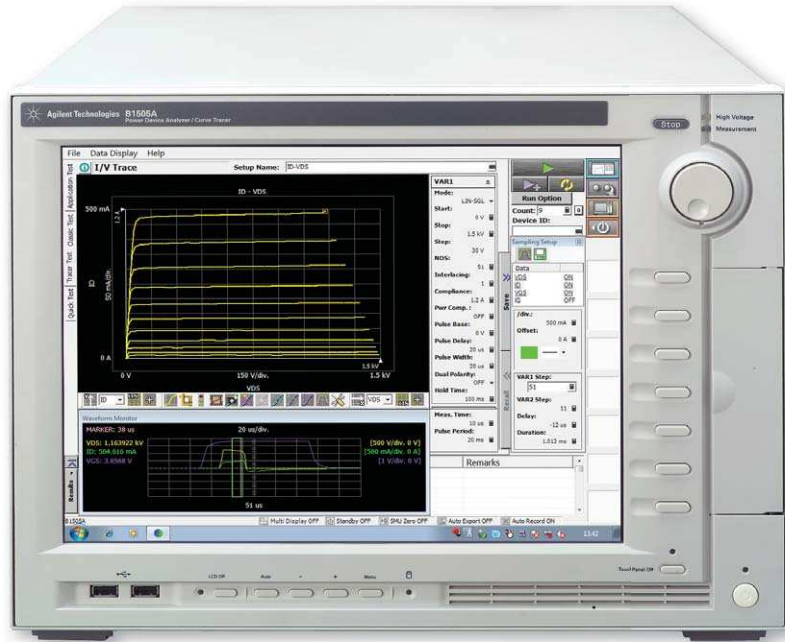

Introduction

The B1505A Power Device Analyzer/ Curve Tracer is a single-box solution with next-generation curve tracer functionality that can accurately evaluate and characterize power devices at up to 10 kV and 1500 amps. The B1505A is capable of handling all types of power device evaluation, with features that include a wide voltage and current range, fast pulsing capability (10 μ s), $\mu\Omega$ level on-resistance measurement resolution and sub-pA level current measurement capability. In addition, an oscilloscope view permits visual verification of both current and voltage pulsed waveforms.

Two independent analog-to-digital (A/D) converters on each channel support a 2 μ s sampling rate for accurate monitoring of the critical timings that can affect device behavior.

It can also perform capacitance measurements at high voltage biases (up to 3000 V). The B1505A with EasyEXPERT software includes a curve tracer mode that combines familiar curve tracer functionality with the convenience of a PC-based instrument; this makes it easy for traditional curve-tracer users to

become productive quickly. Module selector and Quick Test feature enable fully automated measurement on multiple parameters without the need to recable. The net result is improved ease of use, better data analysis and simplified data management for the measurement of power devices and power circuitry.

Anticipate — Accelerate — Achieve



Agilent Technologies

Basic features

- Performs wide range of IV measurements
 - Up to 10 kV / 1500 A
 - Large peak power : 22.5 kW
 - Medium current measurement with high voltage bias (e.g. 500 mA at 1200 V, Peak power : 900 W)
 - $\mu\Omega$ resistance measurement
 - sub-pA leakage measurement
- Performs high bias voltage CV measurements
- Pulsed measurement ($\geq 10 \mu\text{s}$)
- Two independent A/D converters (22 bit equivalent) on each channel enable the simultaneous high-speed (2 μs) sampling of current and voltage
- Temperature measurement
- Easy to use EasyEXPERT test environment
- Curve tracer test mode with knob sweep capability
- Oscilloscope view
- Modular configuration with ten module slots for supported modules
- Multiple SMU types available: HPSMU, MPSMU, HCSMU, MCSMU and HVSMU
- Support for high power devices with up to 6 pins
- Fast high voltage/high current switch for GaN current collapse effect characterization
- Multi-frequency capacitance measurement unit (MFCMU) (1 kHz to 5 MHz) available
- Standard accessories for package test and wafer test: test fixture, module selector and high voltage bias-tee
- 4.2-amp ground unit included standard with the mainframe
- GPIB port for instrument control
- Self-test, self-calibration, diagnostics

Specification conditions

The measurement and output accuracy are specified under the conditions listed below. Note: The SMU measurement and output accuracies are specified at the SMU connector terminals, using the Zero Check terminal as a reference.

1. Temperature: $23 \text{ }^\circ\text{C} \pm 5 \text{ }^\circ\text{C}$
2. Humidity: 20% to 70%
3. Self-calibration after a 40 minute warm-up is required.
4. Ambient temperature change less than $\pm 1 \text{ }^\circ\text{C}$ after self-calibration execution. (Note: This does not apply to the MFCMU).
5. Measurement made within one hour after self-calibration execution. (Note: This does not apply to the MFCMU).
6. Calibration period: 1 year
7. SMU integration time setting:
1 PLC (1 nA to 1 A range, voltage range), 200 μs (20 A range)
Averaging of high-speed ADC:
128 samples per 1 PLC
8. SMU filter: ON (for HPSMU and MPSMU)
9. SMU measurement terminal connection: Kelvin connection (for HPSMU, MPSMU, HCSMU and MCSMU), non-Kelvin (for HVSMU)

Note: This document lists specifications and supplemental characteristics for the B1505A and its associated modules. The specifications are the standards against which the B1505A and its associated modules are tested. When the B1505A or any of its associated modules are shipped from the factory, they meet the specifications. The “supplemental” characteristics described in the following specifications are not guaranteed, but provide useful information about the functions and performance of the instrument.

Note: Module upgrades to existing B1505A systems must be carried out at an Agilent Technologies service centre. In order to ensure system specifications the new modules need to be installed and the complete unit calibrated. Contact your nearest Agilent Technologies office to arrange the installation and calibration of new B1505A modules.

B1505A Specifications

Supported plug-In modules

The B1505A supports ten slots for plug-in modules.

Part number	Description	Slots occupied	Range of operation	Measure resolution
B1510A	High Power Source Monitor Unit (HPSMU)	2	-200 V to 200 V, -1 A to 1 A	2 μ V, 10 fA
B1511A	Medium Power Source Monitor Unit (MPSMU)	1	-100 V to 100 V, -100 mA to 100 mA	0.5 μ V, 10 fA
B1512A	High Current Source Monitor Unit (HCSMU)	2	-40 V to 40 V, -1 A to 1 A -20 V to 20 V, -20 A to 20 A (Pulse only)	200 nV, 10 pA
B1513B	High Voltage Source Monitor Unit (HVSMU)	2	-3000 V to 3000 V, -4 mA to 4 mA -1500 V to 1500 V, -8 mA to 8 mA	200 μ V, 10 fA
B1514A	Medium Current Source Monitor Unit (MCSMU)	1	-30 V to 30 V, -100 mA to 100 mA -30 V to 30 V, -1 A to 1 A (Pulse only)	200 nV, 10pA
B1520A ¹	Multi Frequency Capacitance Measurement Unit (MFCMU)	1	1 kHz to 5 MHz	0.035 fFrms ²

1. N1300A-100 SMU CMU Unify Unit (SCUU) is not supported for the B1505A.

2. Valid when connecting a 10 pF capacitor to the measurement terminals under the following measurement conditions: a frequency of 1 MHz, a signal level of 250 mV AC, and a measurement time of 1 PLC. The display resolution is 0.000001 fF at 1 fF order by 6 digits display.

Maximum module configuration

The total power consumption of all modules cannot exceed 84 W. Under this rule, the B1505A can contain any combination of the following SMUs:

- Up to 4 dual-slot HPSMUs¹
- Up to 10 single-slot MPSMUs
- Up to 2 dual-slot HCSMUs¹
- Up to 6 single-slot MCSMUs
- 1 dual-slot HVSMU

1. The total number of installed HPSMU and HCSMU modules cannot exceed 4.

In addition, up to 1 single-slot MFCMU can be installed per B1505A mainframe for any of the above listed SMU configurations.

The installation order of the modules is: HPSMU, MPSMU, MFCMU, MCSMU, HCSMU and HVSMU starting from the bottom of the B1505A mainframe.

Maximum voltage between Common and Ground

$\leq \pm 42$ V

Ground unit (GNDU) specifications

The GNDU is furnished with the B1505A mainframe.

Output voltage: 0 V \pm 100 μ V
 Maximum sink current: \pm 4.2 A
 Output terminal/connection:
 Triaxial connector, Kelvin
 (remote sensing)

GNDU supplemental characteristics

Load capacitance: 1 μ F

Cable resistance:

For $I_s \leq 1.6$ A: Force line R < 1 Ω
 For 1.6 A < $I_s \leq 2.0$ A: Force line R < 0.7 Ω
 For 2.0 A < $I_s \leq 4.2$ A: Force line R < 0.35 Ω
 For all cases: Sense line R \leq 10 Ω

Where I_s is the current being sunk by the GNDU.

HPSMU Module Specifications

Voltage range, resolution, and accuracy (high resolution ADC)

Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ ±(% + mV)	Maximum current
±2 V	100 µV	2 µV	±(0.018 + 0.4)	±(0.01 + 0.14)	1 A
±20 V	1 mV	20 µV	±(0.018 + 3)	±(0.009 + 0.9)	1 A
±40 V	2 mV	40 µV	±(0.018 + 6)	±(0.01 + 1)	500 mA
±100 V	5 mV	100 µV	±(0.018 + 15)	±(0.012 + 2.5)	125 mA
±200 V	10 mV	200 µV	±(0.018 + 30)	±(0.014 + 2.8)	50 mA

1. ± (% of reading value + offset value in mV)

Current range, resolution, and accuracy (high resolution ADC)

Current range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + A + A)	Measure accuracy ¹ ±(% + A + A)	Maximum voltage
±1 nA	50 fA	10 fA	±(0.1 + 3E-13 + Vo x 1E-15)	±(0.1 + 2E-13 + Vo x 1E-15)	200 V
±10 nA	500 fA	10 fA	±(0.1 + 3E-12 + Vo x 1E-14)	±(0.1 + 1E-12 + Vo x 1E-14)	200 V
±100 nA	5 pA	100 fA	±(0.05 + 3E-11 + Vo x 1E-13)	±(0.05 + 20E-12 + Vo x 1E-13)	200 V
±1 µA	50 pA	1 pA	±(0.05 + 3E-10 + Vo x 1E-12)	±(0.05 + 1E-10 + Vo x 1E-12)	200 V
±10 µA	500 pA	10 pA	±(0.05 + 3E-9 + Vo x 1E-11)	±(0.04 + 2E-9 + Vo x 1E-11)	200 V
±100 µA	5 nA	100 pA	±(0.035 + 15E-9 + Vo x 1E-10)	±(0.03 + 3E-9 + Vo x 1E-10)	200 V
±1 mA	50 nA	1 nA	±(0.04 + 15E-8 + Vo x 1E-9)	±(0.03 + 6E-8 + Vo x 1E-9)	200 V
±10 mA	500 nA	10 nA	±(0.04 + 15E-7 + Vo x 1E-8)	±(0.03 + 2E-7 + Vo x 1E-8)	200 V
±100 mA	5 µA	100 nA	±(0.045 + 15E-6 + Vo x 1E-7)	±(0.04 + 6E-6 + Vo x 1E-7)	200 V ²
±1 A	50 µA	1 µA	±(0.4 + 3E-4 + Vo x 1E-6)	±(0.4 + 15E-5 + Vo x 1E-6)	200 V ²

1. ± (% of reading value + fixed offset in A + proportional offset in A), Vo is the output voltage in V.)

2. 200 V (Io ≤ 50 mA), 100 V (50 mA < Io ≤ 125 mA), 40 V (125 mA < Io ≤ 500 mA), 20 V (500 mA < Io ≤ 1 A), Io is the output current in Amps.

Voltage range, resolution, and accuracy (high speed ADC)

Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ ±(% + mV)	Maximum current
±2 V	100 µV	100 µV	±(0.018 + 0.4)	±(0.01 + 0.7)	1 A
±20 V	1 mV	1 mV	±(0.018 + 3)	±(0.01 + 4)	1 A
±40 V	2 mV	2 mV	±(0.018 + 6)	±(0.015 + 8)	500 mA
±100 V	5 mV	5 mV	±(0.018 + 15)	±(0.02 + 20)	125 mA
±200 V	10 mV	10 mV	±(0.018 + 30)	±(0.035 + 40)	50 mA

1. ±(% of reading value + offset value in mV). Averaging is 128 samples in 1 PLC.

Current range, resolution, and accuracy (high speed ADC)

Current range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + A + A)	Measure accuracy ¹ ±(% + A + A)	Maximum voltage
±1 nA	50 fA	50 fA	±(0.1 + 3E-13 + Vo x 1E-15)	±(0.25 + 3E-13 + Vo x 1E-15)	200 V
±10 nA	500 fA	500 fA	±(0.1 + 3E-12 + Vo x 1E-14)	±(0.25 + 2E-12 + Vo x 1E-14)	200 V
±100 nA	5 pA	5 pA	±(0.05 + 3E-11 + Vo x 1E-13)	±(0.1 + 2E-11 + Vo x 1E-13)	200 V
±1 µA	50 pA	50 pA	±(0.05 + 3E-10 + Vo x 1E-12)	±(0.1 + 2E-10 + Vo x 1E-12)	200 V
±10 µA	500 pA	500 pA	±(0.05 + 3E-9 + Vo x 1E-11)	±(0.05 + 2E-9 + Vo x 1E-11)	200 V
±100 µA	5 nA	5 nA	±(0.035 + 15E-9 + Vo x 1E-10)	±(0.05 + 2E-8 + Vo x 1E-10)	200 V
±1 mA	50 nA	50 nA	±(0.04 + 15E-8 + Vo x 1E-9)	±(0.04 + 2E-7 + Vo x 1E-9)	200 V
±10 mA	500 nA	500 nA	±(0.04 + 15E-7 + Vo x 1E-8)	±(0.04 + 2E-6 + Vo x 1E-8)	200 V
±100 mA	5 µA	5 µA	±(0.045 + 15E-6 + Vo x 1E-7)	±(0.1 + 2E-5 + Vo x 1E-7)	200 V ²
±1 A	50 µA	50 µA	±(0.4 + 3E-4 + Vo x 1E-6)	±(0.5 + 3E-4 + Vo x 1E-6)	200 V ²

1. ±(% of reading value + fixed offset in A + proportional offset in A), Vo is the output voltage in V.)

2. 200 V (Io ≤ 50 mA), 100 V (50 mA < Io ≤ 125 mA), 40 V (125 mA < Io ≤ 500 mA), 20 V (500 mA < Io ≤ 1 A), Io is the output current in Amps.

Power consumption

Voltage source mode:

Voltage range	Power
2 V	$20 \times I_c$ (W)
20 V	$20 \times I_c$ (W)
40 V	$40 \times I_c$ (W)
100 V	$100 \times I_c$ (W)
200 V	$200 \times I_c$ (W)


Where I_c is the current compliance setting.

Current source mode:

Voltage compliance	Power
$V_c \leq 20$	$20 \times I_o$ (W)
$20 < V_c \leq 40$	$40 \times I_o$ (W)
$40 < V_c \leq 100$	$100 \times I_o$ (W)
$100 < V_c \leq 200$	$200 \times I_o$ (W)

Where V_c is the voltage compliance setting and I_o is output current.

HPSMU measurement and output range

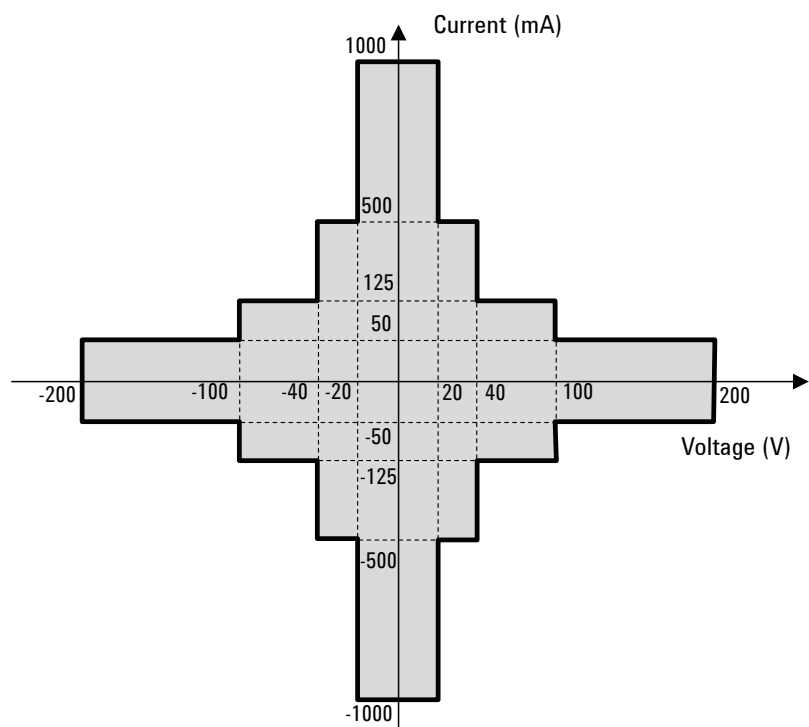

MPSMU Module Specifications

Voltage range, resolution, and accuracy (high resolution ADC)

Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ ±(% + mV)	Maximum current
±0.5 V	25 µV	0.5 µV	±(0.018 + 0.15)	±(0.01 + 0.12)	100 mA
±2 V	100 µV	2 µV	±(0.018 + 0.4)	±(0.01 + 0.14)	100 mA
±5 V	250 µV	5 µV	±(0.018 + 0.75)	±(0.009 + 0.25)	100 mA
±20 V	1 mV	20 µV	±(0.018 + 3)	±(0.009 + 0.9)	100 mA
±40 V	2 mV	40 µV	±(0.018 + 6)	±(0.01 + 1)	²
±100 V	5 mV	100 µV	±(0.018 + 15)	±(0.012 + 2.5)	²

1. ± (% of reading value + offset value in mV)

2. 100 mA ($V_o \leq 20$ V), 50 mA (20 V < $V_o \leq 40$ V), 20 mA (40 V < $V_o \leq 100$ V), V_o is the output voltage in Volts.

Current range, resolution, and accuracy (high resolution ADC)

Current range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + A + A)	Measure accuracy ¹ ±(% + A + A)	Maximum voltage
±1 nA	50 fA	10 fA	±(0.1 + 3E-13 + $V_o \times 1E-15$)	±(0.1 + 2E-13 + $V_o \times 1E-15$)	100 V
±10 nA	500 fA	10 fA	±(0.1 + 3E-12 + $V_o \times 1E-14$)	±(0.1 + 1E-12 + $V_o \times 1E-14$)	100 V
±100 nA	5 pA	100 fA	±(0.05 + 3E-11 + $V_o \times 1E-13$)	±(0.05 + 2E-11 + $V_o \times 1E-13$)	100 V
±1 µA	50 pA	1 pA	±(0.05 + 3E-10 + $V_o \times 1E-12$)	±(0.05 + 1E-10 + $V_o \times 1E-12$)	100 V
±10 µA	500 pA	10 pA	±(0.05 + 3E-9 + $V_o \times 1E-11$)	±(0.04 + 2E-9 + $V_o \times 1E-11$)	100 V
±100 µA	5 nA	100 pA	±(0.035 + 15E-9 + $V_o \times 1E-10$)	±(0.03 + 3E-9 + $V_o \times 1E-10$)	100 V
±1 mA	50 nA	1 nA	±(0.04 + 15E-8 + $V_o \times 1E-9$)	±(0.03 + 6E-8 + $V_o \times 1E-9$)	100 V
±10 mA	500 nA	10 nA	±(0.04 + 15E-7 + $V_o \times 1E-8$)	±(0.03 + 2E-7 + $V_o \times 1E-8$)	100 V
±100 mA	5 µA	100 nA	±(0.045 + 15E-6 + $V_o \times 1E-7$)	±(0.04 + 6E-6 + $V_o \times 1E-7$)	²

1. ± (% of reading value + fixed offset in A + proportional offset in A), V_o is the output voltage in V.)

2. 100 V ($I_o \leq 20$ mA), 40 V (20 mA < $I_o \leq 50$ mA), 20 V (50 mA < $I_o \leq 100$ mA), I_o is the output current in Amps.

Voltage range, resolution, and accuracy (high speed ADC)

Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ ±(% + mV)	Maximum current
±0.5 V	25 µV	25 µV	±(0.018 + 0.15)	±(0.01 + 0.25)	100 mA
±2 V	100 µV	100 µV	±(0.018 + 0.4)	±(0.01 + 0.7)	100 mA
±5 V	250 µV	250 µV	±(0.018 + 0.75)	±(0.01 + 2)	100 mA
±20 V	1 mV	1 mV	±(0.018 + 3)	±(0.01 + 4)	100 mA
±40 V	2 mV	2 mV	±(0.018 + 6)	±(0.015 + 8)	²
±100 V	5 mV	5 mV	±(0.018 + 15)	±(0.02 + 20)	²

1. ±(% of reading value + offset value in mV). Averaging is 128 samples in 1 PLC.

2. 100 mA ($V_o \leq 20$ V), 50 mA (20 V < $V_o \leq 40$ V), 20 mA (40 V < $V_o \leq 100$ V), V_o is the output voltage in Volts.

Current range, resolution, and accuracy (high speed ADC)

Current range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + A + A)	Measure accuracy ¹ ±(% + A + A)	Maximum voltage
±1 nA	50 fA	50 fA	±(0.1 + 3E-13 + $V_o \times 1E-15$)	±(0.25 + 3E-13 + $V_o \times 1E-15$)	100 V
±10 nA	500 fA	500 fA	±(0.1 + 3E-12 + $V_o \times 1E-14$)	±(0.25 + 2E-12 + $V_o \times 1E-14$)	100 V
±100 nA	5 pA	5 pA	±(0.05 + 3E-11 + $V_o \times 1E-13$)	±(0.1 + 2E-11 + $V_o \times 1E-13$)	100 V
±1 µA	50 pA	50 pA	±(0.05 + 3E-10 + $V_o \times 1E-12$)	±(0.1 + 2E-10 + $V_o \times 1E-12$)	100 V
±10 µA	500 pA	500 pA	±(0.05 + 3E-9 + $V_o \times 1E-11$)	±(0.05 + 2E-9 + $V_o \times 1E-11$)	100 V
±100 µA	5 nA	5 nA	±(0.035 + 15E-9 + $V_o \times 1E-10$)	±(0.05 + 2E-8 + $V_o \times 1E-10$)	100 V
±1 mA	50 nA	50 nA	±(0.04 + 15E-8 + $V_o \times 1E-9$)	±(0.04 + 2E-7 + $V_o \times 1E-9$)	100 V
±10 mA	500 nA	500 nA	±(0.04 + 15E-7 + $V_o \times 1E-8$)	±(0.04 + 2E-6 + $V_o \times 1E-8$)	100 V
±100 mA	5 µA	5 µA	±(0.045 + 15E-6 + $V_o \times 1E-7$)	±(0.1 + 2E-5 + $V_o \times 1E-7$)	²

1. ±(% of reading value + fixed offset in A + proportional offset in A), V_o is the output voltage in V.)

2. 100 V ($I_o \leq 20$ mA), 40 V (20 mA < $I_o \leq 50$ mA), 20 V (50 mA < $I_o \leq 100$ mA), I_o is the output current in Amps.

Power consumption

Voltage source mode:

Voltage range	Power
0.5 V	$20 \times I_c$ (W)
2 V	$20 \times I_c$ (W)
5 V	$20 \times I_c$ (W)
20 V	$20 \times I_c$ (W)
40 V	$40 \times I_c$ (W)
100 V	$100 \times I_c$ (W)


Where I_c is the current compliance setting.

Current source mode:

Voltage compliance	Power
$V_c \leq 20$	$20 \times I_o$ (W)
$20 < V_c \leq 40$	$40 \times I_o$ (W)
$40 < V_c \leq 100$	$100 \times I_o$ (W)

Where V_c is the voltage compliance setting and I_o is output current.

MPSMU measurement and output range

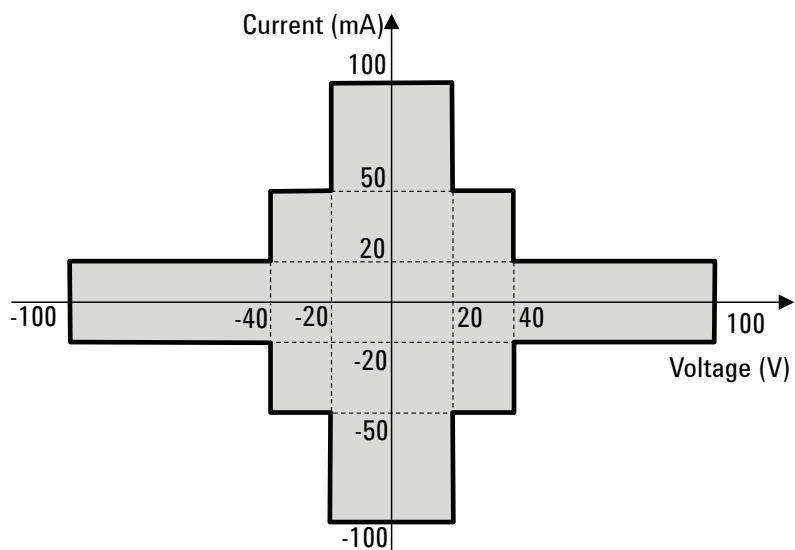

HCSMU Module Specifications

Voltage range, resolution, and accuracy					
Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV + mV)	Measure accuracy ¹ (% + mV + mV)	Maximum current
±0.2 V	200 nV	200 nV	±(0.06 + 0.14 + I _o × 0.05)	±(0.06 + 0.14 + I _o × 0.05)	20 A
±2 V	2 μV	2 μV	±(0.06 + 0.6 + I _o × 0.5)	±(0.06 + 0.6 + I _o × 0.5)	20 A
±20 V	20 μV	20 μV	±(0.06 + 3 + I _o × 5)	±(0.06 + 3 + I _o × 5)	20 A
±40 V	40 μV	40 μV	±(0.06 + 3 + I _o × 10)	±(0.06 + 3 + I _o × 10)	1 A

1. ±(% of reading value + fixed offset in mV + proportional offset in mV). Note: I_o is the output current in A.

Current range, resolution, and accuracy					
Current range	Force resolution	Measure resolution	Force accuracy ¹ (% + A + A)	Measure accuracy ¹ (% + A + A)	Maximum voltage
±10 μA	10 pA	10 pA	±(0.06 + 2E-9 + V _o × 1E-10)	±(0.06 + 2E-9 + V _o × 1E-10)	40 V
±100 μA	100 pA	100 pA	±(0.06 + 2E-8 + V _o × 1E-9)	±(0.06 + 2E-8 + V _o × 1E-9)	40 V
±1 mA	1 nA	1 nA	±(0.06 + 2E-7 + V _o × 1E-8)	±(0.06 + 2E-7 + V _o × 1E-8)	40 V
±10 mA	10 nA	10 nA	±(0.06 + 2E-6 + V _o × 1E-7)	±(0.06 + 2E-6 + V _o × 1E-7)	40 V
±100 mA	100 nA	100 nA	±(0.06 + 2E-5 + V _o × 1E-6)	±(0.06 + 2E-5 + V _o × 1E-6)	40 V
±1 A	1 μA	1 μA	±(0.4 + 2E-4 + V _o × 1E-5)	±(0.4 + 2E-4 + V _o × 1E-5)	40 V
±20 A ²	20 μA	20 μA	±(0.4 + 2E-3 + V _o × 1E-4)	±(0.4 + 2E-3 + V _o × 1E-4)	20 V

1. ±(% of reading value + fixed offset in A + proportional offset in A), V_o is the output voltage in V.

2. Pulse mode only. The maximum value of the base current during pulsing is ±100 mA.

Power consumption

Voltage source mode:

Voltage range	Power
0.2 V	40 × I _c (W)
2 V	40 × I _c (W)
40 V	40 × I _c (W)

Where I_c is the current compliance setting.

For pulse current, I_c = (duty) × I_{pulse}

Current source mode:

Voltage compliance	Power
V _c ≤ 0.2	40 × I _o (W)
0.2 < V _c ≤ 2	40 × I _o (W)
2 < V _c ≤ 40	40 × I _o (W)


Where V_c is the voltage compliance setting and I_o is output current.

For pulse current, I_o = (duty) × I_{pulse}

Current range expansion

If two HCSMUs are combined using the Dual HCSMU combination adapter or the Dual HCSMU Kelvin combination adapter, then the maximum current ranges are 40A (Pulsed) and 2A (DC).

HCSMU measurement and output range

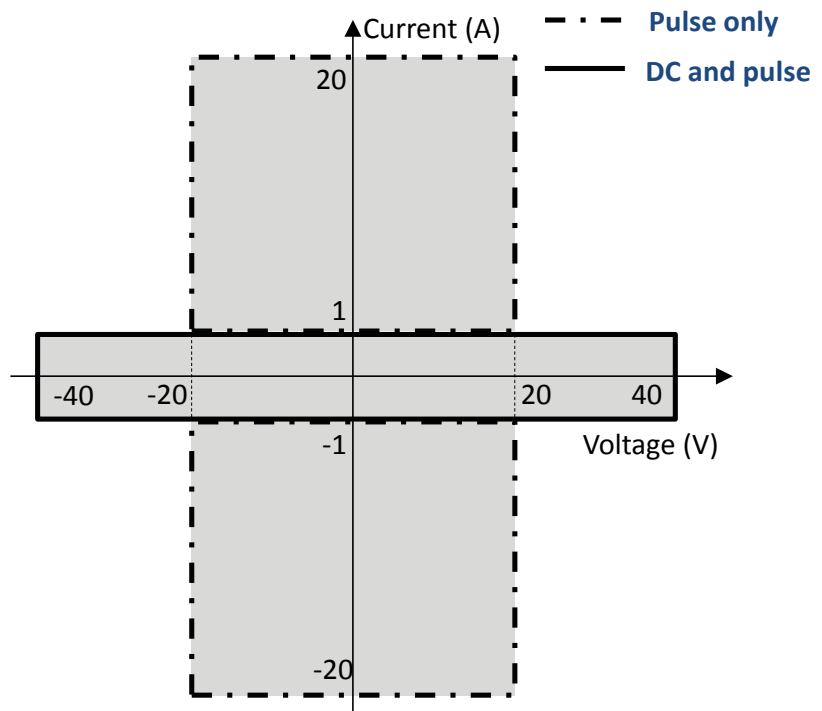

HVSMU Module Specifications

Voltage range, resolution, and accuracy

Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ ±(% + mV)	Maximum current
±200 V	200 μV	200 μV	±(0.03 + 40)	±(0.03 + 40)	8 mA
±500 V	500 μV	500 μV	±(0.03 + 100)	±(0.03 + 100)	8 mA
±1500 V	1.5 mV	1.5 mV	±(0.03 + 300)	±(0.03 + 300)	8 mA
±3000 V	3 mV	3 mV	±(0.03 + 600)	±(0.03 + 600)	4 mA

1. ±(% of reading value + offset voltage V)

Current range, resolution, and accuracy

Current range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + A + A)	Measure accuracy ¹ ±(% + A + A)	Maximum voltage	Minimum set current ²
±1 nA	10 fA	10 fA	±(0.1 + 6E-13 + V _o × 1E-15)	±(0.1 + 6E-13 + V _o × 1E-15)	3000 V	1 pA
±10 nA	100 fA	100 fA	±(0.1 + 25E-13 + V _o × 1E-15)	±(0.1 + 25E-13 + V _o × 1E-15)	3000 V	1 pA
±100 nA	100 fA	100 fA	±(0.05 + 25E-12 + V _o × 1E-13)	±(0.05 + 25E-12 + V _o × 1E-13)	3000 V	100 pA
±1 μA	1 pA	1 pA	±(0.05 + 1E-10 + V _o × 1E-13)	±(0.05 + 1E-10 + V _o × 1E-13)	3000 V	100 pA
±10 μA	10 pA	10 pA	±(0.04 + 2E-9 + V _o × 1E-11)	±(0.04 + 2E-9 + V _o × 1E-11)	3000 V	10 nA
±100 μA	100 pA	100 pA	±(0.03 + 3E-9 + V _o × 1E-11)	±(0.03 + 3E-9 + V _o × 1E-11)	3000 V	10 nA
±1 mA	1 nA	1 nA	±(0.03 + 6E-8 + V _o × 1E-10)	±(0.03 + 6E-8 + V _o × 1E-10)	3000 V	100 nA
±10 mA	10 nA	10 nA	±(0.03 + 2E-7 + V _o × 1E-9)	±(0.03 + 2E-7 + V _o × 1E-9)	1500 V	1 μA

1. ±(% of reading value + fixed offset in A + proportional offset in A), V_o is the output voltage in V.

2. Output current needs to be set more than current shown in the table.

Power consumption

Voltage source mode:

Current compliance	Power
I _c ≤ 4m	3000 × I _c (W)
4m < I _c ≤ 8m	1500 × I _c (W)


Where I_c is the current compliance setting.

Current source mode:

Voltage compliance	Power
V _c ≤ 1500	1500 × I _o (W)
1500 < V _c ≤ 3000	3000 × I _o (W)

Where V_c is the voltage compliance setting and I_o is output current.

HVSMU measurement and output range

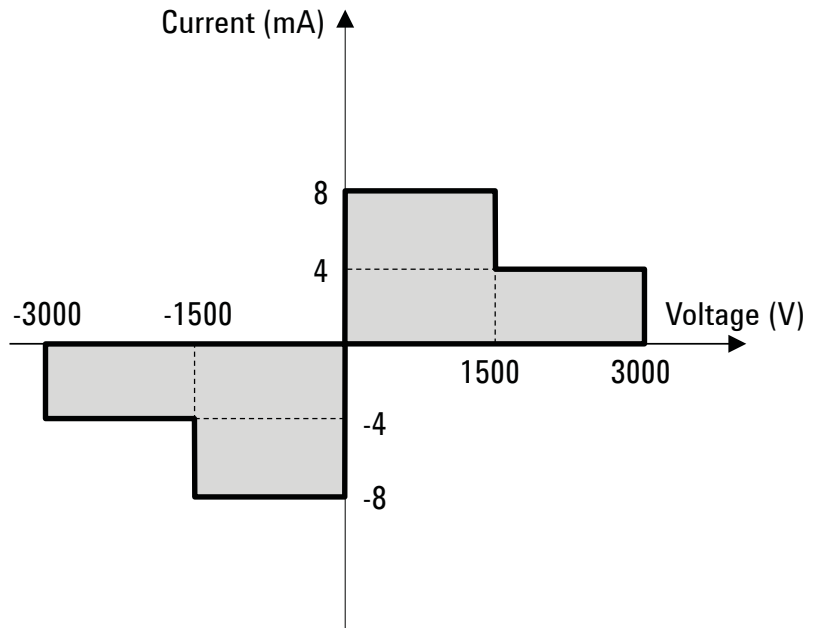

MCSMU Module Specifications

Voltage range, resolution, and accuracy					
Voltage range	Force resolution	Measure resolution	Force accuracy ¹ ±(% + mV)	Measure accuracy ¹ (% + mV + mV)	Maximum current
±0.2 V	200 nV	200 nV	±(0.06 + 0.14)	±(0.06 + 0.14 + I _o × 0.05)	1 A
±2 V	2 μV	2 μV	±(0.06 + 0.6)	±(0.06 + 0.6 + I _o × 0.5)	1 A
±20 V	20 μV	20 μV	±(0.06 + 3)	±(0.06 + 3 + I _o × 5)	1 A
±40 V ²	40 μV	40 μV	±(0.06 + 3)	±(0.06 + 3 + I _o × 10)	1 A

- ±(% of reading value + fixed offset in mV + proportional offset in mV). Note: I_o is the output current in A.
- Maximum output voltage is 30 V.

Current range, resolution, and accuracy					
Current range	Force resolution	Measure resolution	Force accuracy ¹ (% + A + A)	Measure accuracy ¹ (% + A + A)	Maximum voltage
±10 μA	10 pA	10 pA	±(0.06 + 2E-9 + V _o × 1E-10)	±(0.06 + 2E-9 + V _o × 1E-10)	30 V
±100 μA	100 pA	100 pA	±(0.06 + 2E-8 + V _o × 1E-9)	±(0.06 + 2E-8 + V _o × 1E-9)	30 V
±1 mA	1 nA	1 nA	±(0.06 + 2E-7 + V _o × 1E-8)	±(0.06 + 2E-7 + V _o × 1E-8)	30 V
±10 mA	10 nA	10 nA	±(0.06 + 2E-6 + V _o × 1E-7)	±(0.06 + 2E-6 + V _o × 1E-7)	30 V
±100 mA	100 nA	100 nA	±(0.06 + 2E-5 + V _o × 1E-6)	±(0.06 + 2E-5 + V _o × 1E-6)	30 V
±1 A ²	1 μA	1 μA	±(0.4 + 2E-4 + V _o × 1E-5)	±(0.4 + 2E-4 + V _o × 1E-5)	30 V

- ±(% of reading value + fixed offset in A + proportional offset in A), V_o is the output voltage in V.
- Pulse mode only. The maximum value of the base current during pulsing is ±50 mA.

Power consumption

Voltage source mode:

Voltage range	Power
0.2 V	40 × I _c (W)
2 V	40 × I _c (W)
40 V	40 × I _c (W)


Where I_c is the current compliance setting.

Current source mode:

Voltage compliance	Power
V _c ≤ 0.2	40 × I _o (W)
0.2 < V _c ≤ 2	40 × I _o (W)
2 < V _c ≤ 40	40 × I _o (W)

Where V_c is the voltage compliance setting and I_o is output current.

MCSMU measurement and output range

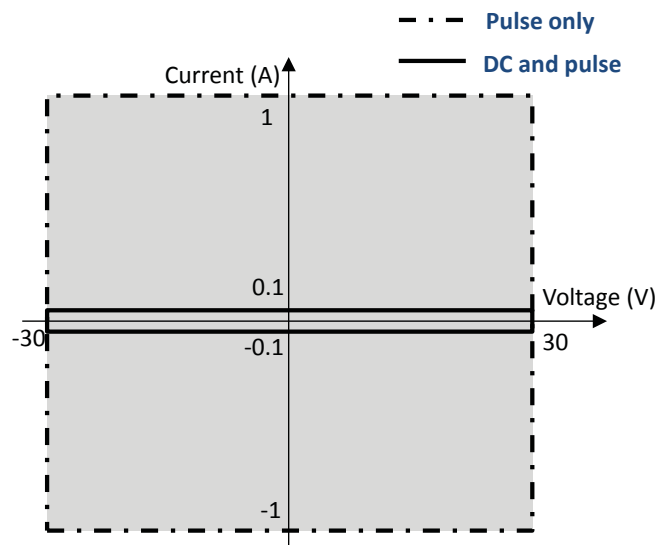

SMU source measurement mode

For HPSMU and MPSMU:

VFIM, IFVM

For HCSPMU, MCSMU and HVSMU:

VFIM, VFVM, IFVM, IFIM

Output terminal/connection:

For HPSMU and MPSMU:

Dual triaxial connector,
Kelvin (remote sensing)

For HCSPMU:

Triaxial connector (for sense) and
coaxial connector (for force)
Kelvin (remote sensing)

For MCSMU:

Dual triaxial connector, Kelvin
(remote sensing)

For HVSMU:

High voltage triaxial connector,
non-Kelvin**Voltage/current compliance** (limiting)The SMU can limit output voltage
or current to prevent damaging the
device under test.

Voltage:

0 V to ± 200 V (HPSMU)0 V to ± 100 V (MPSMU)0 V to ± 40 V (HCSPMU)0 V to ± 30 V (MCSMU)0 V to ± 3000 V (HVSMU)

Current:

 ± 1 pA to ± 1 A (HPSMU) ± 1 pA to ± 100 mA (MPSMU) ± 10 nA to ± 20 A (HCSPMU) ± 10 nA to ± 1 A (MCSMU) ± 1 pA to ± 8 mA (HVSMU)

Compliance accuracy:

Same as the current or voltage set
accuracy.**Power compliance**

For HPSMU:

Power: 0.001 W to 20 W

Resolution: 0.001 W

For MPSMU:

Power: 0.001 W to 2 W

Resolution: 0.001 W

For HCSPMU:

Power: 0.001 W to 40 W (DC)

0.001 W to 400 W (Pulse)

Resolution: 0.001 W

For MCSMU:

Power: 0.001 W to 3 W (DC)

0.001 W to 30 W (Pulse)

Resolution: 0.001 W

For HVSMU:

No power compliance

SMU pulse measurement

Pulse width, period, and delay:

For HPSMU and MPSMU:

Pulse width: 500 μ s to 2 sPulse width resolution: 2 μ s

Pulse period: 5 ms to 5 s

Period \geq delay + width + 2 ms(when delay + width \leq 100 ms)Period \geq delay + width + 10 ms

(when delay + width > 100 ms)

Pulse period resolution: 100 μ s

Pulse delay: 0 s

For HCSPMU:

Pulse width:

50 μ s to 1 ms (20 A range)50 μ s to 2 s (10 μ A to 1 A range)Pulse width resolution: 2 μ s

Pulse period: 5 ms to 5 s

Pulse period resolution: 100 μ s

Pulse duty:

For 20 A range: \leq 1%For 10 μ A to 1 A rangePeriod \geq delay + width + 2 ms(when delay + width \leq 100 ms)Period \geq delay + width + 10 ms

(when delay + width > 100 ms)

Pulse delay: 0 to (Period-width)

For MCSMU:

Pulse width:

10 μ s to 100 ms (1 A range)10 μ s to 2 s (10 μ A to 100 mA
range)Pulse width resolution: 2 μ s

Pulse period: 5 ms to 5 s

Pulse period resolution: 100 μ s

Pulse duty:

For 1 A range: \leq 5%For 10 μ A to 100 mA rangePeriod \geq delay + width + 2 ms(when delay + width \leq 100 ms)Period \geq delay + width + 10 ms

(when delay + width > 100 ms)

Pulse delay: 0 to (Period-width)

For HVSMU:

Pulse width: 500 μ s to 2 sPulse width resolution: 2 μ s

Pulse period: 5 ms to 5 s

Period \geq delay + width + 2 ms(when delay + width \leq 100 ms)Period \geq delay + width + 10 ms

(when delay + width > 100 ms)

Pulse period resolution: 100 μ s

Pulse delay: 0 to (Period – width)

Pulse output limitation:

When the pulse voltage is more
than 1500 volts, the peak and
base of pulse should be same
polarities.

Pulse measurement delay:

2 μ s to (Period – pulse
measurement time – 2 m) s,2 μ s resolution

Supplemental Characteristics

Current compliance setting accuracy (for opposite polarity):

For HPSMU and MPSMU:

For 1 pA to 10 nA ranges:

V/I setting accuracy $\pm 12\%$ of range

For 100 nA to 1 A ranges:

V/I setting accuracy $\pm 2.5\%$ of range

For HCSMU and MCSMU:

For 10 μ A to 1 A ranges:

V/I setting accuracy $\pm 2.5\%$ of range

For 20 A range (HCSMU):

V/I setting accuracy $\pm 0.6\%$ of range

For HVSMU:

For 1 nA to 10 nA ranges:

V/I setting accuracy $\pm 12\%$ of range

For 100 nA to 10 mA ranges:

V/I setting accuracy $\pm 2.5\%$ of range

SMU pulse setting accuracy (fixed measurement range):

For HPSMU and MPSMU:

Width: $\pm 0.5\% \pm 50 \mu$ s

Period: $\pm 0.5\% \pm 100 \mu$ s

For HCSMU and MCSMU:

Width: $\pm 0.1\% \pm 2 \mu$ s

Period: $\pm 0.1\% \pm 100 \mu$ s

For HVSMU:

Width: $\pm 0.1\% \pm 2 \mu$ s

Period: $\pm 0.5\% \pm 100 \mu$ s

Minimum pulse measurement time:

16 μ s (HPSMU and MPSMU)

2 μ s (HCSMU and MCSMU)

6 μ s (HVSMU)

Voltage source output resistance:

(Force line, non-Kelvin connection)

0.2 Ω (HPSMU)

0.3 Ω (MPSMU)

3 Ω (HVSMU, at 10 mA range)

Voltage measurement input resistance:

$\geq 10^{13} \Omega$ (HPSMU, MPSMU)

$\geq 10^9 \Omega$ (HCSMU, MCSMU, ≤ 1 A),
80 k Ω (HCSMU, 20 A)

$\geq 10^{12} \Omega$ (HVSMU)

Current source output resistance:

$\geq 10^{13} \Omega$ (HPSMU, MPSMU)

$\geq 10^9 \Omega$ (HCSMU, MCSMU, ≤ 1 A),
80 k Ω (HCSMU, 20 A)

$\geq 10^{12} \Omega$ (HVSMU, at 10 nA range)

Maximum allowable cable resistance:

(Kelvin connection)

For HPSMU and MPSMU:

Sense: 10 Ω

Force: 10 Ω (≤ 100 mA),

1.5 Ω (>100 mA)

For HCSMU:

Sense: 10 Ω

Force: 0.6 Ω

(with Low Force)

For MCSMU

Sense: 10 Ω

Force : 1 Ω

(with Low Force)

Maximum allowable inductance:

For HCSMU and MCSMU:

Force 3 μ H

(with Low Force (shield))

Maximum load capacitance:

For HPSMU and MPSMU:

1 pA to 10 nA ranges: 1000 pF

100 nA to 10 mA ranges: 10 nF

100 mA and 1 A ranges: 100 μ F

For HCSMU:

10 μ A to 10 mA ranges: 12 nF

100 mA to 20 A ranges: 100 μ F

For MCSMU:

10 μ A to 10 mA range : 12 nF

100 mA to 1 A range : 100 μ F

For HVSMU:

1 nA to 1 μ A ranges: 1000 pF

10 μ A to 10 mA ranges: 10 nF

Maximum guard capacitance:

900 pF (HPSMU and MPSMU)

1500 pF (HVSMU)

Maximum shield capacitance:

5000 pF (HPSMU, MPSMU and

HVSMU)

Noise characteristics:

For HPSMU, MPSMU and HVSMU

Voltage source:

0.01% of V range (rms.)

Current source:

0.1% of I range (rms.)

For HCSMU

Voltage/Current source:

100 mV (0 to peak) max

For MCSMU

Voltage / Current source:

200 mV (0 to peak) max

Overshoot:

For HPSMU and MPSMU

Voltage source: 0.03% of V range

Current source: 1% of I range

For HCSMU and MCSMU (filter ON)

Voltage/Current source:

10% of range

For HVSMU

Voltage source: 1V (resistive load)

Current source: 1% of I range

Range switching transient noise:

For HPSMU and MPSMU (filter ON):

Voltage ranging: 250 mV

Current ranging: 70 mV

For HCSMU and MCSMU:

10 μ A to 1 A ranges:

Voltage ranging: 250 mV

Current ranging: 70 mV

20 A ranges:

Voltage ranging: 5 V max

For HVSMU:

Voltage ranging: 300 mV

Current ranging: 300 mV

Maximum guard offset voltage:

± 1 mV (HPSMU)

± 3 mV (MPSMU)

± 5 mV (HVSMU)

Maximum slew rate:

0.2 V/ μ s (HPSMU and MPSMU)

1 V/ μ s (HCSMU and MCSMU)

0.4 V/ μ s (HVSMU)

Output settling time

For HVSMU:

Output settling time: 500 μ s

To reach 0.01% of settling value.

Conditions:

100 V step, 8 mA compliance,

1000 pF load capacitance

MFCMU (multi frequency capacitance measurement unit) module specifications

Measurement functions

Measurement parameters:

Cp-G, Cp-D, Cp-Q, Cp-Rp, Cs-Rs,
Cs-D, Cs-Q, Lp-G, Lp-D, Lp-Q, Lp-Rp,
Ls-Rs, Ls-D, Ls-Q, R-X, G-B, Z-θ, Y-θ

Ranging:

Auto and fixed

Measurement terminal:

Four-terminal pair configuration,
four BNC (female) connectors

Cable length:

1.5 m or 3 m, automatic
identification of accessories

Test signal

Frequency:

Range: 1 kHz to 5 MHz
Resolution: 1 mHz (minimum)
Accuracy: ±0.008%

Output signal level:

Range: 10 mV_{rms} to 250 mV_{rms}
Resolution: 1 mV_{rms}
Accuracy:

±(10.0% + 1 mV_{rms}) at the
measurement port of the MFCMU
±(15.0% + 1 mV_{rms}) at the
measurement port of MFCMU
cable (1.5 m or 3.0 m)

Output impedance: 50 Ω, typical

Signal level monitor:

Range: 10 mV_{rms} to 250 mV_{rms}
Accuracy:

±(10.0% of reading + 1 mV_{rms})
at the measurement port of the
MFCMU
±(15.0% + 1 mV_{rms})
at the measurement port of
MFCMU cable (1.5 m or 3.0 m)

DC bias function

DC bias:

Range: 0 to ±25 V
Resolution: 1 mV
Accuracy: ±(0.5% + 5.0 mV)
at the measurement port or the
MFCMU or the MFCMU cable
(1.5 m/3 m)

Maximum DC bias current

(Supplemental characteristics):

Impedance measurement range	Maximum DC bias current
50 Ω	10 mA
100 Ω	10 mA
300 Ω	10 mA
1 kΩ	1 mA
3 kΩ	1 mA
10 kΩ	100 μA
30 kΩ	100 μA
100 kΩ	10 μA
300 kΩ	10 μA

Output impedance: 50 Ω, typical

DC bias monitor:

Range: 0 to ±25 V
Accuracy (open load):
±(0.2% of reading + 10.0 mV)
at the measurement port or the
MFCMU cable (1.5 m/3 m)

Sweep characteristics

Available sweep parameters:
Oscillator level, DC bias voltage,
frequency
Sweep type: linear, log
Sweep mode: single, double
Sweep direction: up, down
Number of measurement points:
Maximum 1001 points

Measurement accuracy

The following parameters are used to
express the impedance measurement
accuracy at the measurement port of
the MFCMU or the MFCMU cable
(1.5 m or 3 m).

Z_x : Impedance measurement value (Ω)

D_x : Measurement value of D

$$E = E_p' + (Z_s' / |Z_x| + Y_o' |Z_x|) \times 100 (\%)$$

$$E_p' = E_{PL} + E_{POSC} + E_p (\%)$$

$$Y_o' = Y_{OL} + Y_{OSC} + Y_o (S)$$

$$Z_s' = Z_{SL} + Z_{OSC} + Z_s (\Omega)$$

|Z| accuracy
±E (%)

θ accuracy
±E/100 (rad)

C accuracy
at $D_x \leq 0.1$
±E (%)

$$\text{at } D_x > 0.1 \\ \pm E \times \sqrt{(1 + D_x^2)} (\%)$$

D accuracy
at $D_x \leq 0.1$
±E/100

$$\text{at } D_x > 0.1 \\ \pm E \times (1 + D_x) / 100$$

G accuracy
at $D_x \leq 0.1$
±E / D_x (%)

$$\text{at } D_x > 0.1 \\ \pm E \times \sqrt{(1 + D_x^2)} / D_x (\%)$$

Note: measurement accuracy is speci-
fied under the following conditions:

Temperature: 23 °C ±5 °C
Integration time: 1 PLC

Parameters E_{POSC} Z_{OSC}		
Oscillator level	E_{POSC} (%)	Z_{OSC} (m Ω)
$125 \text{ mV} < V_{OSC} \leq 250 \text{ mV}$	$0.03 \times (250/V_{OSC} - 1)$	$5 \times (250/V_{OSC} - 1)$
$64 \text{ mV} < V_{OSC} \leq 125 \text{ mV}$	$0.03 \times (125/V_{OSC} - 1)$	$5 \times (125/V_{OSC} - 1)$
$32 \text{ mV} < V_{OSC} \leq 64 \text{ mV}$	$0.03 \times (64/V_{OSC} - 1)$	$5 \times (64/V_{OSC} - 1)$
$V_{OSC} \leq 32 \text{ mV}$	$0.03 \times (32/V_{OSC} - 1)$	$5 \times (64/V_{OSC} - 1)$

V_{OSC} is oscillator level in mV.

Parameters E_{PL} Y_{OL} Z_{SL}			
Cable length	E_{PL} (%)	Y_{OL} (nS)	Z_{SL} (m Ω)
1.5 m	$0.02 + 3 \times f/100$	$750 \times f/100$	5.0
3 m	$0.02 + 5 \times f/100$	$1500 \times f/100$	5.0

f is frequency in MHz. If measurement cable is extended, open compensation, short compensation, and load compensation must be performed.

Parameters Y_{OSC} Y_0 E_P Z_S				
Frequency	Y_{OSC} (nS)	Y_0 (nS)	E_P (%)	Z_S (m Ω)
$1 \text{ kHz} \leq f \leq 200 \text{ kHz}$	$1 \times (125/V_{OSC} - 0.5)$	1.5	0.095	5.0
$200 \text{ kHz} < f \leq 1 \text{ MHz}$	$2 \times (125/V_{OSC} - 0.5)$	3.0	0.095	5.0
$1 \text{ MHz} < f \leq 2 \text{ MHz}$	$2 \times (125/V_{OSC} - 0.5)$	3.0	0.28	5.0
$2 \text{ MHz} < f$	$20 \times (125/V_{OSC} - 0.5)$	30.0	0.28	5.0

f is frequency in Hz.

V_{OSC} is oscillator level in mV.

Example of calculated C/G measurement accuracy

Frequency	Measured capacitance	C accuracy ¹	Measured conductance	G accuracy ¹
5 MHz	1 pF	$\pm 0.61\%$	$\leq 3 \mu\text{S}$	$\pm 192 \text{ nS}$
	10 pF	$\pm 0.32\%$	$\leq 31 \mu\text{S}$	$\pm 990 \text{ nS}$
	100 pF	$\pm 0.29\%$	$\leq 314 \mu\text{S}$	$\pm 9 \mu\text{S}$
	1 nF	$\pm 0.32\%$	$\leq 3 \text{ mS}$	$\pm 99 \mu\text{S}$
1 MHz	1 pF	$\pm 0.26\%$	$\leq 628 \text{ nS}$	$\pm 16 \text{ nS}$
	10 pF	$\pm 0.11\%$	$\leq 6 \mu\text{S}$	$\pm 71 \text{ nS}$
	100 pF	$\pm 0.10\%$	$\leq 63 \mu\text{S}$	$\pm 624 \text{ nS}$
	1 nF	$\pm 0.10\%$	$\leq 628 \mu\text{S}$	$\pm 7 \mu\text{S}$
100 kHz	10 pF	$\pm 0.18\%$	$\leq 628 \text{ nS}$	$\pm 11 \text{ nS}$
	100 pF	$\pm 0.11\%$	$\leq 6 \mu\text{S}$	$\pm 66 \text{ nS}$
	1 nF	$\pm 0.10\%$	$\leq 63 \mu\text{S}$	$\pm 619 \text{ nS}$
	10 nF	$\pm 0.10\%$	$\leq 628 \mu\text{S}$	$\pm 7 \mu\text{S}$
10 kHz	100 pF	$\pm 0.18\%$	$\leq 628 \text{ nS}$	$\pm 11 \text{ nS}$
	1 nF	$\pm 0.11\%$	$\leq 6 \mu\text{S}$	$\pm 66 \text{ nS}$
	10 nF	$\pm 0.10\%$	$\leq 63 \mu\text{S}$	$\pm 619 \text{ nS}$
	100 nF	$\pm 0.10\%$	$\leq 628 \mu\text{S}$	$\pm 7 \mu\text{S}$
1 kHz	100 pF	$\pm 0.92\%$	$\leq 63 \text{ nS}$	$\pm 6 \text{ nS}$
	1 nF	$\pm 0.18\%$	$\leq 628 \text{ nS}$	$\pm 11 \text{ nS}$
	10 nF	$\pm 0.11\%$	$\leq 6 \mu\text{S}$	$\pm 66 \text{ nS}$
	100 nF	$\pm 0.10\%$	$\leq 63 \mu\text{S}$	$\pm 619 \text{ nS}$

1. The capacitance and conductance measurement accuracy is specified under the following conditions:

$D_x \leq 0.1$

Integration time: 1 PLC

Test signal level: 30 mV_{rms}

At four-terminal pair port of MFCMU

UHC (Ultra High Current) Expander / Fixture (N1265A) Specifications

Specifications

Functions:

Fixture capability

Current expander capability

Expands the B1505A's current capability up to 1500 A. Current expansion is made using the Ultra High Current Unit (UHCU), which is comprised of an external module and either two MCSMUs, two HCSMUs or one MCSMU and one HCSMU.

Selector capability

This allows the user to switch the output between the UHCU and other modules connected to the selector input ports. The modules supported on the high-voltage input port are the HVSMU and HVMCU; the modules supported on the SMU input port are the HPSMU and MPSMU.

Channels:

Channel	Number	Input	Output
SMU	6 (When using non-Kelvin connections) 3 (When using Kelvin connections)	Triaxial ¹	Banana
UHV	1	UHV coaxial (High), SHV (Low)	UHV coaxial (High), SHV (Low)
Bias Tee	1	SHV x 2(High, Low)	SHV x 2 (High, Low)
Gate control	1	Triaxial x 2 (Force, Sense)	Banana x 2 (High, Low)
Selector	1 ²	HV Triaxial x 1 Triaxial x 2 (Force, Sense)	Banana x 6 (High Force/Sense, Low Force/Sense, Guard, Chassis)

1. Either the HCSMU or the Dual HCSMU can be connected to the SMU 3 port.

2. The UHCU or any module connected to one of the other two selector input terminals can be connected to the output terminal.

Maximum output for selector channel:

HVSMU Output : ± 3000 V/4 mA, ± 1500 V/8 mA

HVMCU Output : ± 2200 V/1.1 A, ± 1500 V/2.5 A

HPSMU Output: ± 200 V/1 A

MPSMU Output: ± 100 V/100 mA

UHCU Output: ± 60 V/1500 A or 500 A

Refer to each module specification.

Gate control channel:

Non-Kelvin connection

Maximum Voltage : ± 40 V

Maximum Current : ± 1 A Pulse, 100m A DC.

Output Resistance: 0 Ω /10 Ω /100 Ω /1000 Ω (nominal value)

UHCU:

Output peak power	
Current range	Peak power
± 500 A	7.5 kW
± 1500 A	22.5 kW

Voltage range, resolution, and accuracy				
Voltage range	Setting resolution	Measure resolution	Setting accuracy ^{1,2,3} ±(% + mV)	Measure accuracy ^{1,3} ±(% + mV)
± 60 V	200 μV	100 μV	±(0.2 + 10)	±(0.2 + 10)

1. ±(% of reading value + fixed offset in mV)
2. Setting accuracy is defined at open load.
3. Accuracy is defined 1ms pulse width at 500A range and 500 μs pulse width at 1500A range.

Current range, resolution, and accuracy ¹				
Current range	Setting resolution	Measure resolution	Setting accuracy ^{2,3} ±(% + A + A)	Measure accuracy ^{2,3} ±(% + A + A)
± 500 A	1 mA	500 μA	±(0.6 + 0.3 + 0.01*Vo)	±(0.6 + 0.3 + 0.01*Vo)
± 1500 A	4 mA	2 mA	±(0.8 + 0.9 + 0.02*Vo)	±(0.8 + 0.9 + 0.02*Vo)

1. Maximum voltage compliance in current pulse mode is 63 V. Over 400 A at 500 A range and over 1200 A at 1500 A range are supplemental characteristics.
2. Accuracy is defined with 1ms pulse width at 500 A range and with 500 μs pulse width at 1500 A range.
3. ±(% of reading value + fixed offset in A + proportional offset in A), Vo is the Output Voltage.

UHCU Pulse width and resolution				
Current range	Voltage pulse width	Current pulse width	Resolution	Pulse period ¹
500 A	10 μsec – 1 msec	10 μsec – 1 msec	2 μsec	Duty ≤ 0.4%
1500 A	10 μsec – 500 μsec	10 μsec – 500 μsec	2 μsec	Duty ≤ 0.1%

1. At continuous maximum current output, the output current may be reduced due to insufficient charging time.

Other functionality

Filter

Filter can be used for UHC output in current mode at 500 A range.

Thermocouple input: 2ea

Two K-type thermocouple inputs

Temperature range: -50 °C to 300 °C.

Other Terminals/Indicators

Digital I/O input: 1ea.

Digital I/O output: 1 ea.

Power indicator: 1ea.

High voltage indicator: 1ea.

Selector indicator: 1ea.

Interlock terminal: 1ea.

Earth terminal: 1ea.

Wrist strap terminal: 1ea.

Supplemental characteristics

UHC Output resistance

Output range	Nominal value
500 A	120 mΩ
1500 A	40 mΩ

Leakage

Selector channel

HVSMU is applied at High Sense terminal: less than 1n A

HPSMU/MPSMU is applied at High Force terminal: less than 10 nA

UHVU channel

Less than 1nA


SMU channel

Less than 1nA

Thermocouple reading accuracy

Temperature range	Accuracy
0°C ≤ T < 100° C	+/-2°C
T ≥ 100° C	+/-5°C
T < 0° C	+/-5°C

UHC measurement and output range

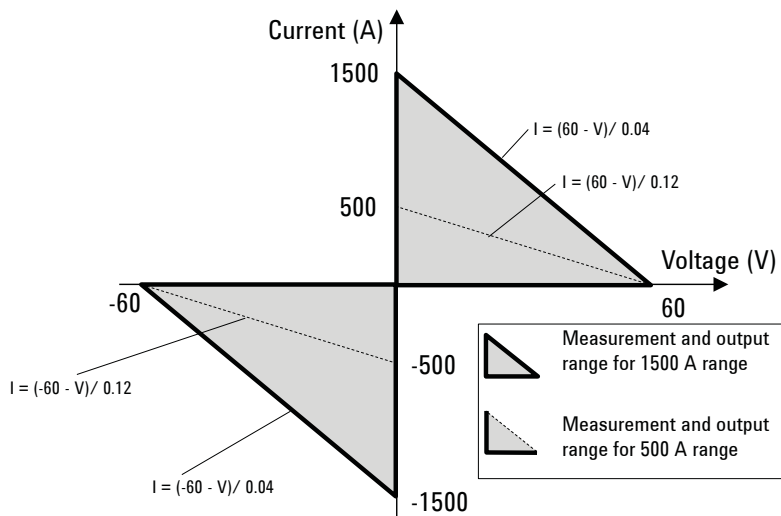

The UHC output is only available in pulsed mode.

In the equations in the above diagram, 'I' stands for current, 'V' for Voltage and 'Rdut' stands for the impedance of the device under test.

HVSMU Current Expander (N1266A) Specifications

Specifications

Functions:

Current expander capability

Expands HVSMU current up to 2.5 A. Current expansion is made using the High Voltage Medium Current Unit (HVMCU), which is comprised of a module in the N1266A, HVSMU and two MCSMUs.

Selector capability

This allows the connections between the output terminal to be switched between the HVMCU and the HVSMU. The HVSMU output can be routed either directly or through a 100 kΩ resistor.

Output Terminals:

High (HV Triaxial)

Low (BNC)

Maximum output:

HVSMU : ±3000 V/4 mA, ±1500 V/8 mA

HVMCU : Refer to HVMCU specification

HVMCU

Output Peak Power	
Voltage range	Peak power
± 2200 V	600 W
± 1500 V	900 W

Voltage range, resolution, and accuracy				
Voltage range	Setting resolution	Measure resolution	Setting accuracy ^{1, 2, 3} ±(% + V)	Measure accuracy ^{1, 2} ±(% + V)
± 2200 V	3 mV	3 mV	±(5 + 20)	±(0.8 + 1.8)
± 1500 V	1.5 mV	3 mV	±(5 + 20)	±(0.8 + 1.8)

1. ±(% of reading value + fixed offset in V)

2. Accuracy is defined with 100 μs pulse at 1.1 A range and 2.5 A range, 1 ms pulse at 100 mA range.

3. Setting accuracy is defined at open load.

Current range, resolution, and accuracy ¹		
Current range	Measure resolution	Measure accuracy ¹ ±(% + A + A)
± 2.5 A	4 μA	±(0.9 + 4E-3 + Vo x 3E-7)
± 1.1 A	4 μA	±(0.9 + 4E-3 + Vo x 3E-7)
± 110 mA	200 nA	±(0.9 + 2E-4 + Vo x 3E-7)

1. Supplemental characteristics over 1.1 A.

HVMCU Pulse width and resolution

Output range	Pulse width	Resolution
1500 V / 2.5 A	10 μsec – 100 μsec	2 μsec
2200 V / 1.1 A	10 μsec – 100 μsec	2 μsec
2200 V / 110 mA	10 μsec – 1 msec	2 μsec

Other Terminals / Indicators

Digital I/O Input: 1ea.
 Digital I/O output: 1ea.
 Power indicator: 1ea
 Selector indicator: 1ea

Supplemental characteristics

HVMCU Charged Capacitance: 0.22 μF


Output resistance

Output range	Nominal value
1500 V / 2.5 A	600 Ω
2200 V / 1.1 A	2000 Ω
2200 V / 110 mA	20000 Ω

Leakage

Selector output
 HVSMU: less than 80 pA

HVMCU Measurement and output range

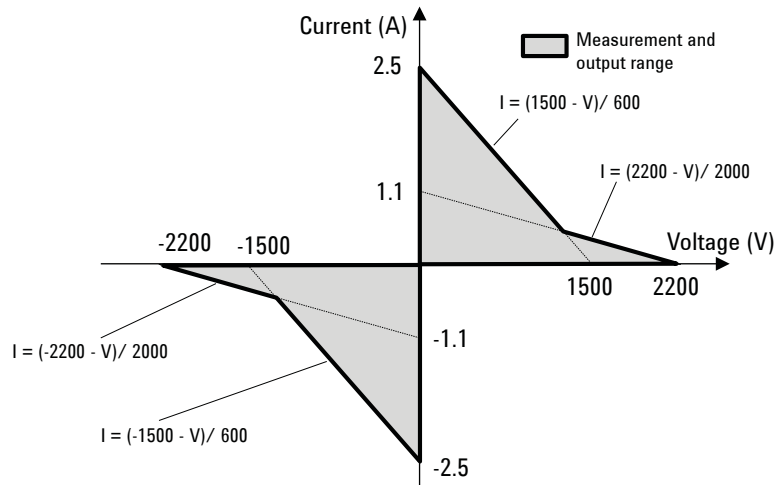

The HVMCU's output is only available in pulsed mode.

In the equations in the above diagram, 'I' stands for current, 'V' for Voltage and 'Rdut' stands for the impedance of the device under test.

UHV (Ultra High Voltage) Expander (N1268A) Specifications

Specifications

Voltage range, resolution, and accuracy ¹				
Voltage range	Force resolution	Measure resolution	Setting accuracy ^{2,3} ±(% + V)	Measure accuracy ² ±(% + V)
± 10 kV	10 mV	10 mV	±(1.2 + 42)	±(1.2 + 42)

1. N1268A is controlled and makes measurement with two MCSMUs or a combination of a HCSMU and a MCSMU.
2. ±(% of reading value + fixed offset in V)
3. Setting accuracy is defined at open load.

Current range, resolution, and accuracy ¹		
Current range	Measure resolution	Measure accuracy ² ±(% + A + A)
± 10 μA	10 pA	±(0.06 + 2E-9 + 1E-9)
± 100 μA	100 pA	±(0.06 + 2E-8 + 1E-9)
± 1 mA	1 nA	±(0.06 + 2E-7 + 1E-9)
± 10 mA	10 nA	±(0.06 + 2E-6 + 1E-9)
± 100 mA ³	100 nA	±(0.06 + 20E-6 + 1E-9)

1. N1268A is controlled and makes measurement with two MCSMUs or a combination of a HCSMU and a MCSMU.
2. ±(% of reading value + fixed offset in A + fixed offset in A)
3. Pulsed mode only (Maximum pulse width is 1 ms). The maximum current is 20 mA.

UHV Pulse width and resolution		
Output range	Pulse width	Resolution
100 mA	100 μs to 1 ms	2 μs
≤ 10 mA	100 μs to 2 s	2 μs

Pulse Period

Min: 10 ms
Max: 5 s

Output Terminals

High : UHV coaxial
Low : SHV

Other Terminals / Indicators


Digital I/O Input: 1ea.
Power indicator: 1ea
High Voltage indicator: 1ea
Interlock terminal Input: 1ea
Interlock terminal Output: 1ea
Earth terminal: 1ea

Supplemental characteristics

UHVU Output resistance	
Output range	Nominal value
High	10000 Ω
Low	1000 Ω

Other AC characteristics	
Slew rate	100 V/μs (with 1m cable)
Overshoot	±1% of setting voltage
Ripple	3 Vp-p
Maximum load capacitance	5 nF
Maximum load inductance	5 μH

UHV measurement and output range

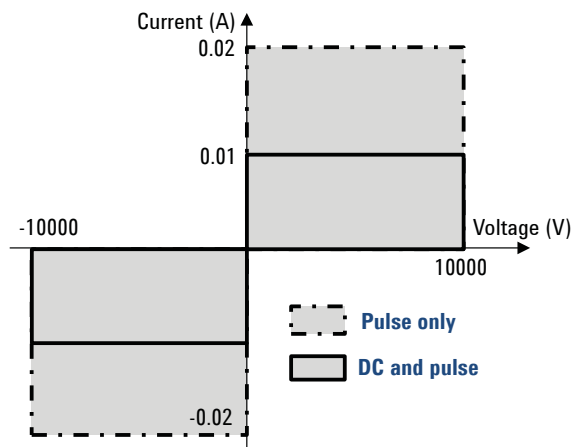

N1267A High Voltage Source Monitor Unit / High Current Source Monitor Unit Fast Switch

Features

The N1267A supports fast switching between the HVSMU and HCSMU to enable the measurement of the Gallium Nitride current collapse effect.

The N1267A switch requires one MCSMU in the B1505A mainframe for control. The gate of the DUT (Device Under Test) can be driven by either an MCSMU or an HCSMU.

Note #1: The N1267A can only be used with the B1513B HVSMU; it cannot be used with the B1513A HVSMU.

Note #2: The N1267A does not support the two HCSMU 40 A configuration.

Note #3: The N1267A does not support the N1265A test fixture/current expander.

Specifications

Input terminals:

HVSMU port, 1ea (HV triaxial)

HCSMU port, 1ea (Force: BNC, Sense: Triaxial)

MCSMU port, 1ea (Force/Sense: Triaxial)

GND port, 1ea (Triaxial)

Output terminals: High (HV triaxial), Low (BNC)

Maximum current: 20 A

Maximum voltage: 3000 V

Measurement mode


GaN Current collapse (Dynamic I-V) measure mode

1. I-V time domain measurement
2. I-V trace measurement

Static characteristics mode

1. I_d - V_{ds} , V_f - I_f measurement
2. $I_d(\text{off})$ - V_{ds} , V_r - I_r measurement

Source and Measure Range

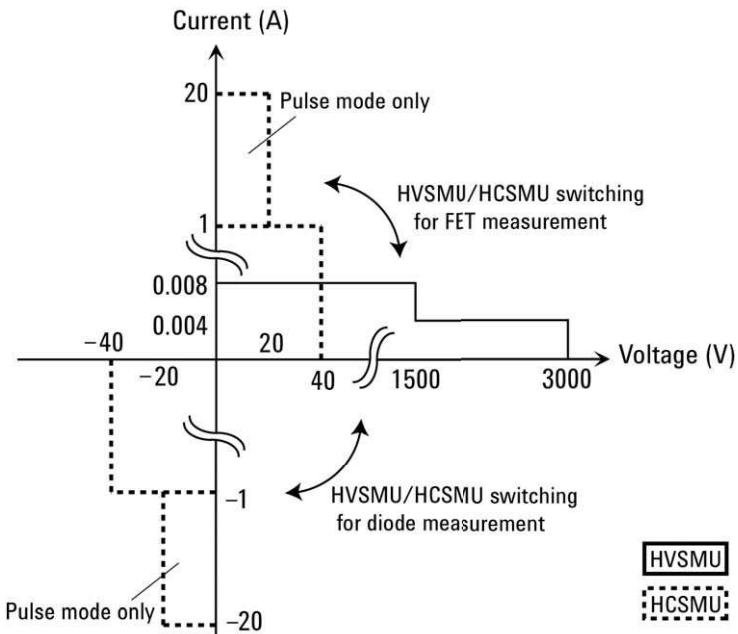

GaN current collapse measure mode

To make the GaN current collapse measurement, the HVSMU first applies high voltage stress to the DUT when the DUT is in the OFF-state. Next the HVSMU performs voltage measurement and the HCSMU performs I-V measurement to monitor the ON-state characteristics of the DUT. When making the ON-state measurement, the HVSMU is measuring voltage and both the HVSMU and HCSMU are used to measure the total current.

HVSMU Source setting range for OFF-state	
Voltage	Current
+1 V - +3000 V ¹⁾	4 mA (V > 1500 V), 8 mA (V ≤ 1500 V)

¹ Setting value must be the ON state voltage plus 1 V or more.

HCSMU source setting range for ON-state		
Voltage	Current	
0 V - ±40 V ²⁾	Maximum	Minimum
	20A pulse (V ≤ 20V) / 1A DC	20 mA ³⁾

² Voltage actually applied to the device under test (DUT) is the setting value minus the voltage drop of the switch.

³ Sum of HCSMU output current and HVSMU output current flow into DUT.

Minimum voltage measurement resolution for OFF-state: 200 µV

Minimum current measurement resolution for ON-state: 100 nA

Minimum transition time (OFF to ON): 20 µs

Duration setting for OFF-state: 10 ms - 655.35

Sampling rate: 2 µs to 12 µs for current, 6 µs for voltage

Minimum ON state duration: 50 µs

Static characteristics mode

The following information applies to measurement of the DUT ON-state static characteristics. The N1267A ensures that the DUT is in the ON-state during these measurements. The HVSMU applies 0 V with 1 µA compliance and measures Vds or Vf. At the same time, the HCSMU is also performing an I-V measurement. The Id or If is determined by adding together the total current measured by both the HCSMU and the HVSMU.

HCSMU source setting for Id-Vds, Vf-If measurement		
Voltage	Current	
0 V - ±40 V)	Maximum	Minimum
	20A pulse (V ≤ 20V) / 1A DC	20 mA ⁴⁾

Minimum voltage measurement resolution: 200 µV

Minimum current measurement resolution: 10 pA ⁴⁾

⁴ Offset error for the Id-Vds, If-Vf measurement is typical 1 µA

The following information applies to measurement of the DUT OFF-state static characteristics. The N1267A ensures that the DUT is in the OFF-state during these measurements. The HCSMU applies 0 V. At the same time, the HVSMU performs I-V measurement and measures Vds or Vr. The Id(Off) or Ir is determined by adding together the total current measured by both the HCSMU and the HVSMU.

HVSMU source setting for Id(off)-Vds, Vr-Ir measurement		
Voltage	Current	
0 V - +3000V	Maximum	Minimum
	4 mA (V > 1500 V), 8 mA (V ≤ 1500 V)	10 µA ⁵⁾

Minimum voltage measurement resolution: 200 µV

Minimum current measurement resolution: 10 pA ⁵⁾

⁵ Leak error for the Idss, Ir-Vr measurement is typical 2 nA.

Accessories

N1258A module selector

Specifications

Input terminals:

HPSMU force port¹, 1 ea., (Triaxial)
HPSMU sense port¹, 1 ea., (Triaxial)
HCSMU force port, 1 ea. (BNC)
HCSMU sense port, 1 ea. (Triaxial)
HVSMU port², 1 ea. (HV triaxial)
GNDU port, 1 ea. (Triaxial)
Digital I/O port, 1 ea. (D-sub 25 pin)
AC power line connector, 1 ea.

1. Either HPSMU or MPSMU can be connected to HPSMU port.
2. Either HVSMU or HVMCU can be connected to HVSMU port.

Output terminal:

High force (HV triaxial)
High sense (HV triaxial)
Low force (BNC)
Low sense (BNC)
External relay control output
(D-sub 25 pin)

Protection:

HPSMU, GNDU, HCSMU Low Force

Power indicator:

LED turns yellow when AC power is applied and turns green the module selector is ready to use.

Status indicator:

Green LED lights to indicate the present connection path of module selector; Open, HCSMU, HPSMU, or HVSMU.

Maximum voltage/current:

For HPSMU port:
±200 V/1 A

For HCSMU port:
±40 V/2 A, ±20 V/30 A
(Pulse width 1 ms, duty 1%)

For HVSMU port:
±3000 V/4 mA,
±1500 V/2.5 A, ±2200 V/1.1 A

Supplemental characteristics

Leakage current:

For HPSMU:
10 pA at 200 V

For HCSMU:
100 pA at 10 V (High Force to Low Force, High Sense to Low Sense)

For HVSMU:
10 pA at 1500 V (humidity range: 20% to 70% RH)
20 pA at 3000 V (humidity range: 20% to 50% RH)

N1259A test fixture

Specifications

Input terminals:

HPSMU port¹, 2 ea.
Force, sense (Triaxial)
HCSMU port, 2 ea.
Force (BNC), sense (Triaxial)
HVSMU port², 1 ea. (HV triaxial)
GNDU port, 1 ea. (Triaxial)
AUX port, 2 ea. (BNC)
Interlock port, 1 ea.

1. Either HPSMU or MPSMU can be connected to HPSMU port.
2. Either HVSMU or HVMCU can be connected to HVSMU port.

Protection:

HPSMU, GNDU, HCSMU Low Force terminal

High voltage indicator:

LED turns red when a SMU output voltage is over 42 V.

Maximum voltage/current:

For HPSMU port:
Force: ±200 V/1 A
Sense: ±200 V

For HCSMU port:
High Force: ±40 V/2 A, ±20 V/40 A (Pulse width 1 ms, duty 1%)
Low Force: ±40 V/2 A, ±20 V/40 A (Pulse width 1 ms, duty 1%)
High Sense: ±40 V
Low Sense: ±40 V

For HVSMU port:

Force: ±3000 V/4 mA,
±1500 V/2.5 A, ±2200 V/1.1 A

Note: The total power consumption of all modules cannot exceed 50 W when using test fixture under the condition that operating temperature is more than 35 °C.

Supplemental characteristics

Leakage current:

For HPSMU (Force, Sense) port:
10 pA at 200 V (Force, Sense)

For HCSMU (High Force, High sense) port: 100 pA at 10 V

For HVSMU (Force) port:
10 pA at 1500 V (humidity range: 20% to 70% RH)
20 pA at 3000 V (humidity range: 20% to 50% RH)

N1259A-010 inline package socket module (3 pin)

Specifications

Number of terminal:

Sockets, 6 ea. (Ø4 mm jack (banana))

DUT interface:

Inline package socket (3-pin)

Maximum voltage for terminals:
3000 Vdc

N1259A-011 universal socket module

Specifications

Number of terminal:

Sockets, 8 ea. (Ø4 mm jack (banana))

Maximum voltage for terminals:
3000 Vdc

N1259A-013 Curve Tracer test adapter socket module

Specifications

Number of terminals:

Sockets, 6 ea.
(Ø4 mm jack (banana))

Test adapter interface:*

Sockets, 6 ea.
(Ø4 mm jack (banana))

Maximum voltage at terminals:

3000V Vdc

Maximum current for terminals:

For Collector/Drain Force and
Emitter/Source Force
39 A (DC), 500 A (Pulse)

For others

1A (DC), 20 A (Pulse)

*A test adapter for Tektronix curve tracers (370B/371B) can be connected to this interface.

N1259A-020 high voltage bias-tee

Specifications

Input terminals:

DC bias input, 1 ea.
(Ø4 mm jack (banana))

MFCMU port, 1 ea.

Hcur, Hpot, Lcur, Lpot, (BNC)

Guard input, 1ea (Ø4 mm banana jack)

Output terminal:

MFCMU port

High (SHV)

Low (SHV)

External DC bias voltage: ± 3000 V

Frequency:

10 kHz to 1 MHz (150 Ω at 10 kHz)

Series capacitance: 110 nF $\pm 5\%$

Input resistance: 100 k Ω $\pm 1\%$

N1259A-021 1 M Ω resistor box

Specifications

Input/output terminals:

Ø4 mm jack (banana), 1 ea.

Resistance: 1 M Ω $\pm 5\%$

Maximum voltage: ± 3000 V

Power rating: 9 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1259A-022 100 k Ω resistor box

Specifications

Input/output terminals:

Ø4 mm jack (banana), 1 ea.

Resistance: 100 k Ω $\pm 5\%$

Maximum voltage: ± 3000 V

Power rating: 6.4 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1259A-030 1 k Ω resistor box for gate

Specifications

Input/output terminals:

Ø4 mm jack (banana), 1 ea.

Resistance: 1 k Ω $\pm 10\%$

Maximum voltage: ± 200 V

Maximum power: 1 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1259A-035 Universal resistor box

Specifications

Input/output terminals:

Ø4 mm banana jack, 1 ea.

Resistance: Installed by a user

Maximum voltage for terminals:

± 3000 V

N1259A-300 module selector for test fixture

Specifications

Input terminals:

HPSMU port¹, 1 ea.

Force, sense (Triaxial)

HCSMU port, 1 ea.

Force (BNC), sense (Triaxial)

HVSMU port², 1 ea. (HV triaxial)

GNDU port, 1 ea. (Triaxial)

Digital I/O port, 1 ea. (D-sub 25 pin)

AC power line connector, 1 ea.

1. Either HPSMU or MPSMU can be connected to HPSMU port.

2. Either HVSMU or HVMCU can be connected to HVSMU port.

Output terminal:

High force and guard

High sense and guard

Low force

Low sense

(Ø4 mm jack (banana))

Protection:

HPSMU, GNDU, HCSMU Low Force

Power indicator:

LED turns yellow when AC power is applied and turns green the module selector is ready to use.

Status indicator:

Green LED lights to indicate the present connection path of module selector; Open, HCSMU, HPSMU, or HVSMU.

Maximum voltage/current:

For HPSMU port:

± 200 V/1 A

For HCSMU port:

± 40 V/2 A, ± 20 V/30 A

(Pulse width 1 ms, duty 1%)

For HVSMU:

± 3000 V/4 mA,

± 1500 V/2.5 A, ± 2200 V/1.1 A

Supplemental characteristics

Leakage current:

For HPSMU:

10 pA at 200 V

For HCSMU:

100 pA at 10 V (High Force to Low Force, High Sense to Low Sense)

For HVSMU:

10 pA at 1500 V (humidity range: 20% to 70% RH)

30 pA at 3000 V (humidity range: 20% to 50% RH)

N1260A high voltage bias-tee

Specifications

Input terminals:

HVSMU port, 1 ea. (HV triaxial)

MFCMU port, 1 ea.

(4 BNC, Hp, Hc, Lp, Hc)

Output terminal:

H-AC Guard (SHV connector)

L-AC Guard (SHV connector)

External DC bias voltage: ± 3000 V

Frequency:

10 kHz to 1 MHz (150 Ω at 10 kHz)

Series capacitance: 110 nF $\pm 5\%$

Input resistance: 100 k Ω $\pm 1\%$

N1261A protection adapter

N1261A-001 protection adapter for HPSMU (triaxial output)

Specifications

Input terminals:

Force (Triaxial)

Sense (Triaxial)

Output terminals:

Force (Triaxial)

Sense (Triaxial)

1. Either the HPSMU or the MPSMU can be connected to HPSMU port.

Supplemental characteristics

Leakage current: 10 pA at 200 V

N1261A-002 protection adapter for GNDU (BNC output)

Specifications

Input terminals:

Force/Sense (Triaxial)

Output terminals:

Force (BNC)

Sense (BNC)

N1261A-003 protection adapter for HPSMU (HV triaxial output)

Specifications

Input terminals¹:

Force (Triaxial)

Sense (Triaxial)

Output terminals:

Force (HV triaxial)

Sense (HV triaxial)

1. Either the HPSMU or the MPSMU can be connected to HPSMU port.

Supplemental characteristics

Leakage current: 10 pA at 200 V

N1261A-004 protection adapter for GNDU (SHV output)

Specifications

Input terminals:

Force/Sense (Triaxial)

Output terminals:

Force (SHV)

Sense (SHV)

N1262A Resistor Box

N1262A-001 1 M Ω resistor box

Specifications

Input terminals:

HVSMU port, 1 ea. (HV triaxial)

Output terminals:

SHV connector, 1 ea.

Resistance: 1 M Ω $\pm 5\%$

Maximum voltage: ± 3000 V

Maximum power: 9 W

Supplemental characteristics

Leakage current:

10 pA at 100 V

N1262A-002 100 k Ω resistor box

Specifications

Input terminals:

HVSMU port, 1 ea. (HV triaxial)

Output terminals:

SHV connector, 1 ea.

Resistance: 100 k Ω $\pm 5\%$

Maximum voltage: ± 3000 V

Maximum power: 6.4 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1262A-010 1 k Ω resistor box for gate (triaxial output)

Specifications

Input terminals:

Triaxial connector, 1 ea.

Output terminals:

Triaxial connector, 1 ea.

Resistance: 1 k Ω $\pm 10\%$

Maximum voltage: ± 200 V

Maximum power: 1 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1262A-011 1 k Ω resistor box for gate (SHV output)

Specifications

Input terminals:

HV triaxial connector, 1 ea.

Output terminals:

SHV connector, 1 ea.

Resistance: 1 k Ω $\pm 10\%$

Maximum voltage: ± 3000 V

Maximum power: 1 W

Supplemental characteristics

Leakage current: 10 pA at 100 V

N1262A-020 Universal resistor box, Triaxial

Specifications

Input terminals:

Triaxial connector, 1 ea.

Output terminals:

Triaxial connector, 1 ea.

Resistance: Installed by user

Maximum voltage for terminals: ± 200 V

N1262A-021 Universal resistor box, HV Triaxial to SHV

Specifications

Input terminals:

HVSMU port, 1 ea. (HV triaxial)

Output terminals:

SHV connector, 1 ea.

Resistance: Installed by user

Maximum voltage for terminals:
 ± 3000 V

N1262A-023 Universal resistor box for Ultra High Voltage

Specifications

Input terminals:

UHV coaxial connector, 1 ea.

Output terminals:

UHV coaxial connector, 1 ea.

Resistance: Installed by user

Maximum voltage for terminals:
 ± 10 kV

N1262A-036 50 Ohm Termination Adapter

Specifications

Input terminal (BNC)

Output terminal (BNC)

Maximum power: 1 W

Accessories for N1265A

N1254A-524 500 A Ultra High Current Prober System Cable

Specifications

Input terminals: 8 ea. ($\emptyset 4$ mm jack (banana))

Selector Output

High Force

High Sense

Low Force

Low Sense

Guard

Gate output

High Force

Low Force

Chassis

Output terminals

High Force ($\emptyset 4$ mm jack (banana))

Low Force ($\emptyset 4$ mm jack (banana))

High Sense (HV triaxial)

Low Sense (BNC)

Gate (BNC)

Maximum voltage / current

For High Force

± 3000 V / 39 A (DC), 500 A (Pulse)

For Low Force

± 200 V / 39 A (DC), 500 A (Pulse)

For High Sense

± 3000 V / 1 A

For Low Sense, Gate

± 200 V / 1 A

N1265A-010 500 A Ultra High Current 3-pin Inline Package Socket Module

Specifications

Number of terminal:

Sockets, 6 ea. ($\emptyset 4$ mm jack (banana))

DUT interface:

Inline package socket (3-pin)

Maximum voltage for terminals:

3000 Vdc

Maximum current for terminals:

For Force

39 A (DC), 500 A (Pulse)

For sense

1A (DC), 20 A (Pulse)

N1265A-011 Universal Socket Module

Specifications

Number of terminal:

Sockets, 6 ea. ($\emptyset 4$ mm jack (banana))

Maximum voltage for terminals:
3000 Vdc

Universal blank area :

90 mm (W) x 81 mm (D)

N1265A-013 Curve Tracer Test Adapter Socket Module

Specifications

Number of terminals: Sockets, 6 ea. ($\emptyset 4$ mm jack (banana))

Test adapter interface:*

Sockets, 6 ea. ($\emptyset 4$ mm jack (banana))

Maximum voltage at terminals:
3000V Vdc

Maximum current for terminals:

For Collector/Drain Force and Emitter/Source Force

39 A (DC), 500 A (Pulse)

For others

1A (DC), 20 A (Pulse)

*A test adapter for Tektronix curve tracers (370B/371B) can be connected to this interface.

N1265A-035 Universal R-Box for N1265A

Specifications

Input: 4 ea. ($\emptyset 4$ mm plug (banana))

High (Force, Sense)

Low (Force, Sense)

Output terminals: 2 ea. ($\emptyset 4$ mm jack (banana))

High, Low

Resistance: Installed by a user

Maximum voltage for terminals: ± 200 V

N1265A-040 10 kV Ultra High Voltage Gate Protection Adapter

Specifications

Input: 4 ea. (Ø4 mm plug (banana))
High (Force, Sense)
Low (Force, Sense)
Output terminals: 2 ea. (Ø4 mm jack (banana))
High, Low
Maximum voltage: ±200 V
Maximum surge voltage: ±10 kV

N1265A-041 Thermocouple, Type K, 2 ea

Feature

N1265A-041 can be connected to Thermocouple terminal inside the N1265A and enables B1505A to read out temperature at the top of the thermocouple.

Specifications

Connector: Type K plug
Length: 3000 mm
Temperature range: -50 °C to +180 °C

N1265A-045 Container for Protection Adapter and Bias Tee

Feature

N1265A-045 can accommodate protection adapters and bias tee which are used with N1265A to make the measurement environment clean and safe

Specifications

Dimension: 420 mm W x 193 mm H x 565 mm D
Weight: 15 kg
Maximum superimposed load: 50 kg

N1269A Ultra High Voltage Connection Adapter

Feature

To make the connection simple and to protect measurement resources from unexpected surge when connecting UHVU to wafer prober.

Specifications

Input terminals:
Gate MCSMU Force, 1ea (Triaxial)
Gate MCSMU Sense, 1ea (Triaxial)
Chuck MCSMU Force, 1ea (Triaxial)
Chuck MCSMU Sense, 1ea (Triaxial)
UHV Low, 1ea (HV triaxial)
Output terminals: 3ea (SHV)
Gate, Chuck, Source
Maximum voltage: ±200 V
Maximum surge voltage: ±10 kV

Agilent EasyEXPERT Software

Functions

Operation mode:
Application test mode, Classic test mode, Tracer test mode (Curve tracer mode), Oscilloscope view, Quick test mode

Key features:

- Categorized and predefined application library
- Device definition
- Measurement parameter settings
- Save/Recall My Favorite Setups
- Define/customize application library
- Execute measurement (Single/Repeat/Append)
- Oscilloscope view
- Quick test execution
- Direct control
- Save/Recall measurement data and settings
- Test result data management
- Import/Export device definition, measurement settings, my favorite setup, measurement data, and application library
- Graph plot display/analysis/printing
- Workspace management
- Self-test, self calibration, diagnostics

Application library

Category:

Sample test definitions for the following applications. They are subject to change without notice.
High Power Device, Utility

Measurement mode details

The Agilent B1505A supports the following measurement modes:

- IV spot
- IV staircase sweep
- IV pulsed spot
- IV pulsed sweep
- IV staircase sweep with pulsed bias
- IV Sampling
- IV High speed sampling
- Multi channel sweep*
- Multi channel pulse spot
- Multi channel pulse sweep
- CV sweep
- C-t sampling
- C-f sweep
- CV (DC bias) staircase sweep
- List sweep
- Linear search**
- Binary search**

* EasyEXPERT supports VAR1 and VAR1'.

**They are supported by FLEX command only.

Each SMU can sweep using VAR1 (primary sweep), VAR2 (secondary sweep), or VAR1' (synchronous sweep).

VAR1

Primary sweep controls the staircase (dc or pulsed) voltage or current sweep.

Maximum number of steps: $N_1=1001$

VAR2

Subordinate linear staircase or linear pulsed sweep. After primary sweep is completed, the VAR2 unit output is incremented.

Maximum number of steps: $N_2=1001$
(condition: $1 \leq N_1 \times N_2 \leq 128128$)

VAR1

Staircase or pulse sweep synchronized with the VAR1 sweep. Sweep is made with a user specified ratio and offset value. VAR1' output is calculated as $VAR1' = a \times VAR1 + b$, where "a" is the user specified ratio and "b" is the user specified offset value.

CONST

A source unit can be set as a constant voltage or current source depending on the unit.

Sweep measurement time settings:

Hold time:

0 to 655.35 s, 10 ms resolution

Delay time:

0 to 65.5350 s, 100 μ s resolution
(Staircase sweep, multi channel sweep)

0 to 655.350 s, 100 μ s resolution
(CV(DC bias) staircase sweep, AC level sweep, frequency sweep)

Step delay time:

0 to 1 s, 100 μ s resolution

Step output trigger delay time:

0 to (delay time) s, 100 μ s resolution

Step measurement trigger delay time:

0 to 65.535 s, 100 μ s resolution

Staircase sweep measurement mode:

Forces swept voltage or current, and measures DC voltage or current. One channel can sweep current or voltage while up to ten channels can measure current or voltage. A second channel can be synchronized with the primary sweep channel as an additional voltage or current sweep source.

Number of steps: 1 to 1001

Sweep type: linear or logarithmic

Sweep direction:

Single or double sweep

Pulsed sweep measurement mode:

Forces pulsed swept voltage or current, and measures DC voltage or current. A second channel can be programmed to output a staircase sweep voltage or current synchronized with the pulsed sweep output.

Staircase sweep with pulsed bias measurement mode:

Forces swept voltage or current, and measures DC voltage or current. A second channel can be programmed to output a pulsed bias voltage or current. A third channel can be synchronized with the primary sweep channel as an additional voltage or current sweep source.

Sampling (time domain) measurement mode

Displays the time sampled voltage/current data (by SMU) versus time.

Sampling points:

For linear sampling:

1 to 100,001/(number of channels)

For log sampling:

1 to 1 + (number of data for 11 decades)

Sampling mode: linear, log

Sampling interval range:

100 μ s to 2 ms, 10 μ s resolution

2 ms to 65.535 s, 1 ms resolution

For < 2 ms, the interval is

$\geq 100 \mu\text{s} + 20 \mu\text{s} \times (\text{num. of channels} - 1)$

Hold time, initial wait time:

-90 ms to -100 μ s, 100 μ s resolution

0 to 655.35 s, 10 ms resolution

Measurement time resolution: 100 μ s

Oscilloscope View (I/V):

Displays the time sampled current or voltage data for the HCSPMU, MCSMU, HVSMU, UHCU, HVMCU and UHVU modules versus time. The window over which the measurement is being performed is also displayed, permitting verification of measurement timing over the output waveform.

Sampling interval :

2 μ s (HCSPMU/MCSMU/UHCU/HVMCU/UHVU)

6 μ s (HVSMU)

Sampling points:

2000 Sa (HCSPMU/MCSMU/UHCU/HVMCU/UHVU)

4000 Sa (HVSMU)

Marker function :

Read-out for each data channel

Resolution : 2 μ s

Data saving :

Numeric: Text/CSV/XMLSS

Image: EMF/BMP/JPG/PNG

Search measurement mode:

Forces and measures voltage or current by using linear search method or binary search method.

Bias hold function

This function allows you to keep a source active between measurements. The source module will apply the specified bias between measurements when running classic tests inside an application test, in quick test mode, or during a repeated measurement. The function ceases as soon as these conditions end or when a measurement that does not use this function is started.

Current offset cancel

This function subtracts the offset current from the current measurement raw data, and returns the result as the measurement data. This function is used to compensate the error factor (offset current) caused by the measurement path such as the measurement cables, manipulators, or probe card.

Time stamp

The B1505A supports a time stamp function utilizing an internal quartz clock.

Resolution: 100 μ s

Other measurement characteristics

Measurement Control:

Single, Repeat, Append, and Stop

SMU Setting Capabilities:

Limited auto ranging, voltage/current compliance, power compliance, automatic sweep abort functions, self-test, and self-calibration

Arithmetic and analysis functions

User functions

Up to 20 user-defined functions can be defined using arithmetic expressions.

Measured data and pre-defined variables can be used in the computation. The results can be displayed on the LCD.

Arithmetic operators

+, -, *, /, ^, abs (absolute value), at (arc tangent), avg (averaging), cond (conditional evaluation), delta, diff (differential), exp (exponent), integ (integration), lgt (logarithm, base 10), log (logarithm, base e), mavg (moving average), max, min, sqrt, trigonometric function, inverse trigonometric function, and so on.

Physical constants

Keyboard constants are stored in memory as follows:

q: Electron Charge, 1.602177 E-19 C

k: Boltzman's Constant, 1.380658 E-23

ϵ (e): Dielectric Constant of Vacuum, 8.854188 E-12

Engineering units

The following unit symbols are also available on the keyboard:

a (10^{-18}), f (10^{-15}), p (10^{-12}), n (10^{-9}), u or μ (10^{-6}), m (10^{-3}), k (10^3), M (10^6), G (10^9), T (10^{12}), P (10^{15})

Analysis capabilities

Overlay graph comparison

A graphics plot can be stored and overlaid.

Scale

Auto scale and zoom

Marker

Marker to min/max, interpolation, direct marker, and marker skip

Cursor

Direct cursor

Line

Two lines, normal mode, grad mode, tangent mode, and regression mode

Automatic analysis function

On a graphics plot, the markers and lines can be automatically located using the auto analysis setup. Parameters can be automatically determined using automatic analysis, user function, and read out functions.

Data variable display

Up to 20 user-defined parameters can be displayed on the graphics screen.

Analysis functions

Up to 20 user-defined analysis functions can be defined using arithmetic expressions.

Measured data, pre-defined variables, and read out functions can be used in the computation. The results can be displayed on the LCD.

Read out functions

The read out functions are built-in functions for reading various values related to the marker, cursor, or line.

Graph plot

Display mode

Data display window can be printed.

Only X-Y graph can be printed.

Graph plot file

Graph plot can be stored as image data to clip board or mass storage device.

File type: bmp, gif, png, emf

Output

Display modes

X-Y graph, list display, and parameter display

X-Y graph display

X-axis and up to eight Y-axis

Linear and log scale

Real time graph plotting

List display

Measurement data and calculated user function data are listed in conjunction with VAR1 step number or time domain sampling step number. Up to 20 data sets can be displayed.

Other functions

Import/export files.

File type:

Agilent EasyEXPERT format, XML-SS format, CSV format

Data storage

Hard disk drive, DVD-ROM/CD-R/CD-RW drive

Interfaces

GPIB, Interlock, USB

(USB 2.0, front 2, rear 2),

LAN (100BASE-TX/10BASE-T),

trigger in/out, digital I/O

Trigger I/O

Only available using GPIB FLEX commands.

Trigger in/out synchronization pulses before and after setting and measuring dc voltage and current. Arbitrary trigger events can be masked or activated independently.

Supported external instruments

EasyEXPERT Standard edition:

- Supported by application tests: 4284A/E4980A, 81110A, 3458A

EasyEXPERT Plus edition:

- All external instruments supported by EasyEXPERT Standard edition

Furnished software

- Prober control execution files
- Desktop EasyEXPERT software with license-to-use for Standard edition
- 4155/56 setup file converter tool

(Supported operating systems:

Microsoft® Windows® XP

Professional (Service Pack 3 or

later), Windows Vista Business

(Service Pack 2 or later (32bit

only)), and Windows 7 Professional

(Service Pack 1 or later (32bit

and 64bit)); Supported language:

English (US))

General specifications

Temperature range

Operating: +5 °C to +40 °C

Storage: -20 °C to +60 °C

Humidity range¹

Operating: 20% to 70% RH, non-condensing

Storage: 10% to 90% RH, non-condensing

Storage: 20% to 80% RH, non-condensing (N1268A)

Altitude

Operating: 0 m to 2,000 m (6,561 ft)

Storage: 0 m to 4,600 m (15,092 ft)

0 m to 2,000 m (6,561 ft) (N1268A)

Power requirement

ac Voltage: 90 V to 264 V

Line Frequency: 47 Hz to 63 Hz

Maximum volt-amps (VA)

B1505A: 900 VA

N1258A: 65VA

N1259A-300: 35VA

N1265A: 400 VA

N1266A: 60 VA

N1268A: 350 VA

Acoustic Noise Emission

Lpa < 70 dB

About measurement accuracy

RF electromagnetic field and SMU measurement accuracy:

SMU voltage and current measurement accuracy can be affected by RF electromagnetic field strengths greater than 3 V/m in the frequency range of 80 MHz to 1 GHz. The extent of this effect depends upon how the instrument is positioned and shielded.

Induced RF field noise and SMU measurement accuracy:

SMU voltage and current measurement accuracy can be affected by induced RF field noise strengths greater than 3 V_{rms} in the frequency range of 150 kHz to 80 MHz. The extent of this effect depends upon how the instrument is positioned and shielded.

Regulatory compliance

EMC:

IEC 61326-1 / EN 61326-1

Canada: ICES/NMB-001

AS/NZS CISPR 11

Safety:

IEC61010-1 / EN 61010-1

CAN/CSA-C22.2 No. 61010-1

Certification

CE, cCSAus, C-Tick

Dimensions

B1505A:

420 mm W x 330 mm H x 575 mm D

N1258A module selector:

330 mm W x 120 mm H x 410 mm D

N1259A test fixture:

420 mm W x 272 mm H x 410 mm D

N1260A High voltage bias-tee:

164 mm W x 53 mm H x 125 mm D

N1261A-001 HPSMU protection adapter (Triaxial output):

80 mm W x 40 mm H x 110 mm D

N1261A-002 GNDU protection adapter (BNC output):

80 mm W x 40 mm H x 110 mm D

N1261A-003 HPSMU protection adapter (HV triaxial output):

90 mm W x 40 mm H x 140 mm D

N1261A-004 GNDU protection adapter (SHV output):

80 mm W x 40 mm H x 125 mm D

N1262A resistor box:

50 mm W x 40 mm H x 125 mm D

N1265A UHC expander / fixture:

420 mm W x 285 mm H x 575 mm D

N1266A HVSMU current expander:

420 mm W x 75 mm H x 575 mm D

N1267A HVSMU / HCSMU fast switch:

202 mm W x 56 mm H x 175 mm D

N1268A UHV expander:

420 mm W x 222 mm H x 482 mm D

Weight

B1505A (empty): 20 kg

B1511A: 1.1 kg

B1510A: 2.0 kg

B1512A: 2.1 kg

B1513B: 2.0 kg

B1514A: 1.3 kg

B1520A: 1.3 kg

N1258A: 5.0 kg

N1259A: 12.0 kg

N1260A: 0.6 kg

N1261A: 0.3 kg

N1262A: 0.3 kg

N1265A: 30 kg

N1266A: 10 kg

N1267A: 0.8 kg

N1268A: 18 kg

N1268A: 0.4 kg

Furnished accessories

Measurement cables and adapter

Triaxial cable for HPSMU, MPSMU and MCSMU, 2 ea.

HCSMU cable, 1 ea.

HCSMU Kelvin adapter, 1 ea.

HVSMU cable, 1 ea.

Interlock cable, 1 ea.

Ground unit cable, 1 ea.

Keyboard, 1 ea.

Mouse, 1 ea.

Stylus pen, 1 ea.

Power cable, 1 ea.

Manual CD-ROM, 1 ea.

Desktop EasyEXPERT CD-ROM, 1 ea.

License-to-use for Desktop EasyEXPERT Standard edition, 1 license

Software CD-ROM

(including utility tools)

Disk set for Agilent

4155B/4155C/4156B/4156C

firmware update, 1 set

SMU number label for the B1505A

installed with SMU, 1 sheet

N1258A : Digital I/O cable, 1 ea.

N1259A-300 : Digital I/O cable, 1 ea.

N1265A : Digital I/O cable, 1 ea.

N1266A : Digital I/O cable, 1 ea.

N1268A : Digital I/O cable, 1 ea.,

Interlock cable, 1 ea.

¹ In case of some supplemental characteristics, humidity range is defined as 20% to 50% RH

Order Information

Mainframe and modules

B1505A	Power Device Analyzer/Curve Tracer mainframe
	Configure the following modules: High power SMU (HPSMU) Medium power SMU (MPSMU) High current SMU (HCSMU) Medium current SMU (MCSMU) High voltage SMU (HVSMU) Multi frequency CMU (MFCMU)
B1505A-015	1.5 m cable
B1505A-030	3.0 m cable
B1505A-050	50 Hz line frequency
B1505A-060	60 Hz line frequency
B1505A-A6J	ANSI Z540 compliant calibration
B1505A-UK6	Commercial calibration certificate with test data
B1505A-ABA	English documentation
B1505A-ABJ	Japanese documentation
B1500A-1CM	Rackmount kit

B1505A expanders/fixtures

N1259A	Test fixture
N1259A-010	Inline package socket module (3 pin)
N1259A-011	Universal socket module
N1259A-012	Blank PTFE board
N1259A-013	Curve Tracer test adaptor socket module
N1259A-020	High voltage bias-tee
N1259A-021	1 M Ω Resistor box
N1259A-022	100 k Ω Resistor box
N1259A-030	1 k Ω Resistor box for gate
N1259A-035	Universal R-Box
N1259A-300	Module selector
N1265A	UHC expander / fixture
N1265A-010	500 A Ultra High Current 3-pin Inline Package Socket Module
N1265A-011	Universal Socket Module
N1265A-013	Curve Tracer Test Adapter Socket Module
N1265A-015	1500 A Current Option
N1265A-035	Universal R-Box for N1265A
N1265A-040	10 kV Ultra High Voltage Gate Protection Adapter
N1265A-041	Thermocouple, Type K, 2 ea
N1265A-045	Container for Protection Adapter and Bias Tee
N1266A	High Voltage Source Monitor Unit Current Expander
N1267A	High Voltage Source Monitor Unit / High Current Source Monitor Unit Fast Switch
N1268A	Ultra High Voltage Expander

B1505A accessories

16444A-001	Keyboard
16444A-002	Mouse
16444A-003	Stylus pen
N1253A-100	Digital I/O cable
N1253A-200	Digital I/O BNC box
N1254A-100	Ground unit Kelvin adapter
N1254A-101	Triaxial(m)-BNC(f)
N1254A-102	Triaxial(m)-BNC(m)
N1254A-103	Triaxial(m)-BNC(f)
N1254A-104	Triaxial(f)-BNC(m)
N1254A-105	Triaxial(f)-BNC(m)
N1254A-106	Triaxial(m)-BNC(f)
N1254A-107	Triaxial(m)-BNC(f)
N1254A-500	HV Jack Connector (Solder Type)
N1254A-501	HV Jack / Jack Adapter
N1254A-502	HV plug Connector(Solder Type)
N1254A-503	BNC Coax Cable Assy 1.5m(Open End)
N1254A-504	HVTriax Jack Coax Cable Assy 1.5m(Open End)
N1254A-505	HVTriax Plug Triax Cable Assy 1.5m (Open End)
N1254A-506	HVTriax Plug Coax Cable Assy 1.5m(Open End)
N1254A-507	HVTriax Plug Coax Cable Assy 1.5m
N1254A-508	Test Lead cable Black
N1254A-509	Test Lead cable Red
N1254A-510	Dolphin clip 2 ea. (red and black)
N1254A-511	Cable lag adapter 2 ea. (red and black)
N1254A-512	SHV Cable Assy 250mm
N1254A-513	SHV to Banana
N1254A-514	BNC-Plug Plug
N1254A-515	BNC-Jack-Plug-Jack
N1254A-516	BNC-Jack-Jack-Jack
N1254A-517	Adapter, Triaxial Jack to Triaxial Plug
N1254A-518	SHV Cable 1.5 m
N1254A-520	10 kV Ultra High Voltage Open End Cable, 1 m.
N1254A-521	10 kV Ultra High Voltage Jack to Jack Adapter
N1254A-522	1500 A Ultra High Current Banana to Banana Cable, 2 ea.
N1254A-523	1500 A Ultra High Current Banana to Open End Cable, 1 m, 2 ea
N1254A-524	500 A Ultra High Current Prober System Cable
N1258A	Module selector
N1260A	High voltage bias-tee
N1261A	Protection adapter
N1262A	Resistor box
N1262A-020	Universal R-Box, Triaxial
N1262A-021	Universal R-Box, HV Triaxial to SHV
N1262A-023	Universal R-Box for Ultra High Voltage
N1262A-036	50 Ohm Termination Adapter

Order Information

SMU cables/accessories

16493S-001	HCSMU cable (1.5 m)
16493S-002	HCSMU cable (3 m)
16493S-010	HCSMU Kelvin adapter
16493S-011	HCSMU non-Kelvin adapter
16493S-020	Dual HCSMU Kelvin combination adapter
16493S-021	Dual HCSMU combination adapter
16493T-001	High voltage triaxial cable (1.5 m)
16493T-002	High voltage triaxial cable (3 m)
16493U-001	High current BNC cable (1.5 m)
16493U-002	High current BNC cable (3 m)
16494A-001	Triaxial cable (1.5 m)
16494A-002	Triaxial cable (3 m)
16493K-001	Kelvin triaxial cable (1.5 m)
16493K-002	Kelvin triaxial cable (3 m)
16493V-001	10 kV Ultra High Voltage Cable, 1.5 m
16493V-002	10 kV Ultra High Voltage Cable, 3 m
N1269A	Ultra High Voltage Connection Adapter

CMU accessories

N1300A-001	CMU cable (1.5 m)
N1300A-002	CMU cable (3 m)

Other accessories

16493G-001	Digital I/O cable (1.5 m)
16493G-002	Digital I/O cable (3 m)
16493J-001	Interlock cable (1.5 m)
16493J-002	Interlock cable (3 m)
16493L-001	GNDU cable (1.5 m)
16493L-002	GNDU cable (3 m)

Retrofit and upgrade kits

B1505AU	Upgrade kit for B1505A
B1505AU-001	Conversion kit from B1500A to B1505A
B1505AU-010	High power source monitor unit (B1510A)
B1505AU-011	Medium power source monitor unit (B1511A)
B1505AU-012	High current source monitor unit (B1512A)
B1505AU-013	High voltage source monitor unit (B1513B)
B1505AU-014	Medium current source monitor unit (B1514A)
B1505AU-020	Multi frequency capacitance measurement unit (B1520A)
B1505AU-SWS	EasyEXPERT Extension support and subscription
N1259AU	Upgrade kit for N1259A
N1265AU	Upgrade kit for N1265A

Package solution

B1505AP	Pre-configured Power Device Analyzer/Curve Tracer (B1505A w/ modules/fixture)
B1505AP-H20	3 kV / 20 A / Fixture Pack
B1505AP-H21	3 kV / 20 A / C-V / Fixture Pack
B1505AP-H50	3 kV / 500 A / Fixture Pack
B1505AP-H51	3 kV / 500 A / C-V / Fixture Pack
B1505AP-H70	3 kV / 1500 A / Fixture Pack
B1505AP-H71	3 kV / 1500 A / C-V / Fixture Pack
B1505AP-U50	10 kV / 500 A / Fixture Pack
B1505AP-U70	10 kV / 1500 A / Fixture Pack



Agilent Email Updates

www.agilent.com/find/emailupdates
Get the latest information on the products and applications you select.

Agilent Channel Partners

www.agilent.com/find/channelpartners
Get the best of both worlds: Agilent's measurement expertise and product breadth, combined with channel partner convenience.



Agilent Advantage Services is committed to your success throughout your equipment's lifetime. To keep you competitive, we continually invest in tools and processes that speed up calibration and repair and reduce your cost of ownership. You can also use Infoline Web Services to manage equipment and services more effectively. By sharing our measurement and service expertise, we help you create the products that change our world.

www.agilent.com/find/advantageservices



www.agilent.com/quality



Agilent B1500A Semiconductor Device Analyzer

www.agilent.com/find/B1500A



Agilent B2900A Series Precision Source/Measure Unit

www.agilent.com/find/B2900A

www.agilent.com
www.agilent.com/find/b1505a

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at:

www.agilent.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	(11) 4197 3600
Mexico	01800 5064 800
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 112 929
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 375 8100

Europe & Middle East

Belgium	32 (0) 2 404 93 40
Denmark	45 45 80 12 15
Finland	358 (0) 10 855 2100
France	0825 010 700*
	*0.125 €/minute
Germany	49 (0) 7031 464 6333
Ireland	1890 924 204
Israel	972-3-9288-504/544
Italy	39 02 92 60 8484
Netherlands	31 (0) 20 547 2111
Spain	34 (91) 631 3300
Sweden	0200-88 22 55
United Kingdom	44 (0) 118 927 6201

For other unlisted countries:

www.agilent.com/find/contactus

Revised: January 6, 2011

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 2012
Published in USA, September 13, 2012
5990-3853EN



Agilent Technologies