




# MIPI DigRF v4 (M-PHY) Protocol Triggering and Decode for Infiniium Series Oscilloscopes

## Data Sheet

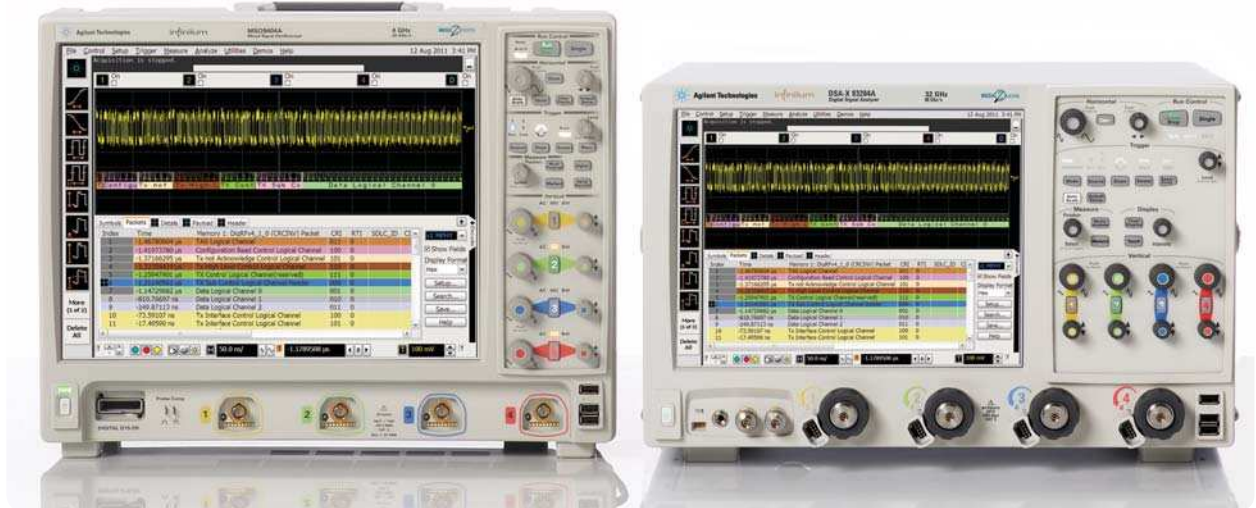

### This application is available in the following license variations.

- Order N8807A for a user-installed license
- Order option 051 for a factory-installed license with new 9000, 90000 or 90000 X Series oscilloscopes
- Order N5435A option 047 for a server-based license that works on 9000, 90000 and 90000 X Series oscilloscopes



# MIPI DigRF v4 (M-PHY)

MIPI (Mobile Industry Processor Interface) serial buses are the backbone for communication in mobile products. The serial bus interface provides content-rich points for debug and test. However, since these protocols transfer bits serially, using a traditional oscilloscope has limitations. Manually converting captured 1's and 0's to protocol requires significant effort, can't be done in real-time, and includes potential for human error. As well, traditional scope triggers are not sufficient for specifying protocol-level conditions.

Extend your scope capability with Agilent's MIPI DigRF v4 (M-PHY) triggering and decode application. This application makes it easy to debug and test designs that include MIPI DigRF v4 buses using your Infiniium Series oscilloscope.

- Set up your scope to show MIPI DigRF v4 protocol decode in less than 30 seconds.
- Get access to a rich set of integrated protocol-level triggers.
- Save time and eliminate errors by viewing packets at the protocol level.
- Use time-correlated views to quickly troubleshoot serial protocol problems back to their timing or signal integrity root cause.

The following are the MIPI DigRF v4 protocols and features that will be supported by the application.

1. Supports DigRF v4 v1.00.00 decode and triggering
2. Decodes high-speed (HS-BURST) and low-speed (SYS-BURST) modes
3. Decodes with and without cyclical redundancy check (CRC) support
4. Supports decode on Tx and Rx packets
5. Supports search capability for various frames, sequence and errors



### Easy to find

Turn decode on/off via the "Serial Decode" button on the front of 9000 Series scopes or in the "Setup" menu. View decode embedded on the waveform display or in the protocol viewer listing window. (See pages 4-5.)



### 30 Second MIPI Setup

Configure your oscilloscope to display protocol decode in under 30 seconds. Use "Auto Setup" to automatically configure sample rate, memory depth, threshold and trigger levels.




### Support for live and saved waveforms

Perform and view decode information on both live and saved waveforms. Decode up to any combination of 4 live or saved waveforms.

## MIPI DigRF v4 (M-PHY) setup, protocol triggering, and search capabilities

Get access to a rich set of integrated protocol-level triggers. The application includes a suite of configurable protocol-level trigger conditions specific to MIPI DigRF v4. When serial triggering is selected, the application uses software-based triggering.

With software-based protocol triggering, the oscilloscope takes signals acquired using either scope or digital channels and reconstructs protocol frames after each acquisition. It then inspects these protocol frames against specified protocol-level trigger conditions and triggers when the condition is met.

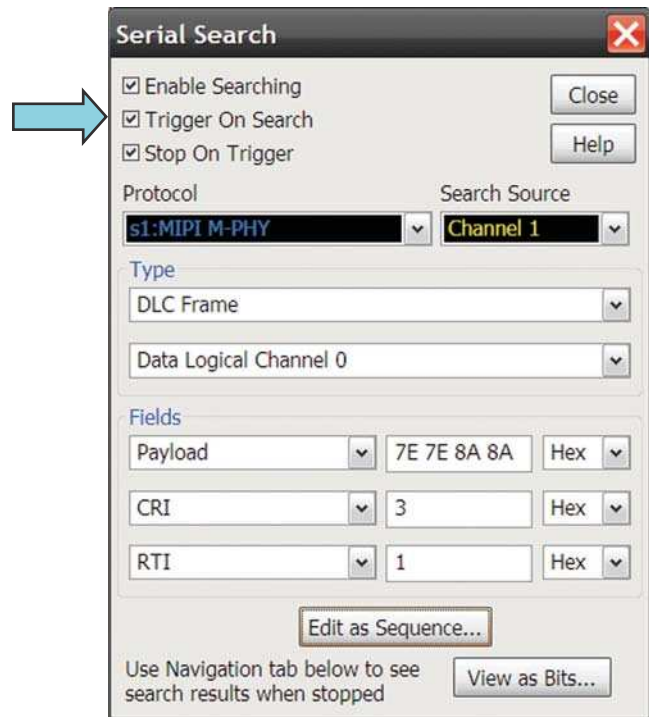



### MIPI trigger and search setup

Quickly access the software-based trigger via the trigger or search menus. Software-based triggering enables quick setup of data, remote, or error frames.

# MIPI DigRF v4 (M-PHY) protocol decode

Get access to a rich set of integrated protocol-level triggers. The application includes a suite of configurable protocol-level trigger conditions specific to MIPI DigRF v4. When serial triggering is selected, the application uses software-based triggering.

With software-based protocol triggering, the oscilloscope takes signals acquired using scope channels and reconstructs protocol frames after each acquisition. It then inspects these protocol frames against specified protocol-level trigger conditions and triggers when the condition is met.

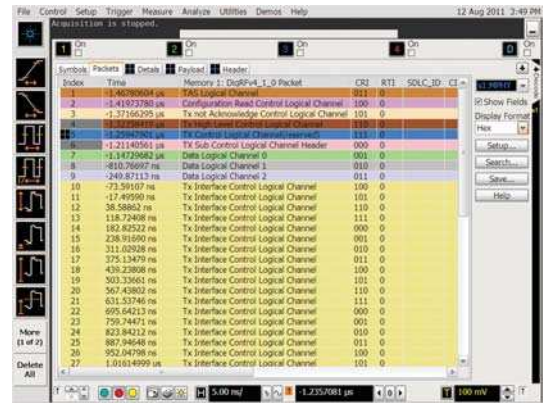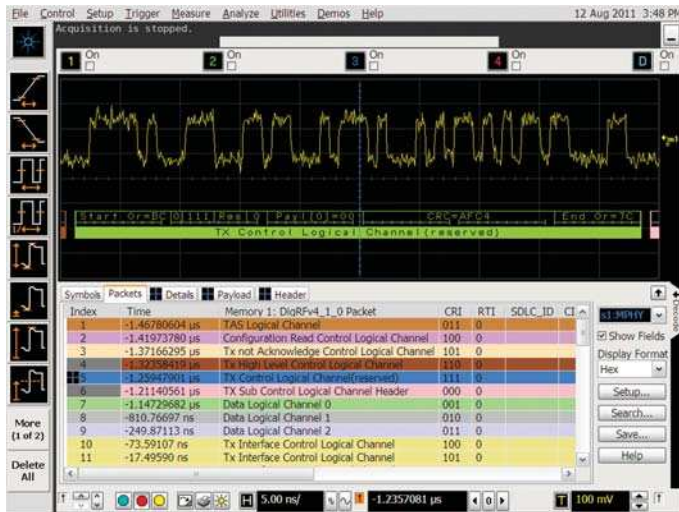

Compact protocol using the full screen listing.

The protocol viewer window shows the index number, time stamp value identifier, packet type, and data values for each MIPI DigRF v4 packet. Data in the listing window can be saved to a .csv or .txt file for off-line.

Quickly move between physical and MIPI DigRF v4 protocol layer information using the time-correlated tracing marker. Display protocol content using embedded decode in the waveform area. Or, see protocol events in a compact listing format. Minor tick marks indicate clock transitions. Major tick marks indicate segments of the serial packet MIPI DigRF v4 measurements are automatically time-correlated with measurement on other scope channels.




MIPI DigRF v4 decode embedded in waveform area

Utilize the oscilloscope waveform area to display decode information. Minor ticks indicate clock transitions and major ticks show segments within each MIPI DigRF v4 packet.



### Using multiple scopes?

Server-based licensing allows users to borrow an application for a specified period of time.

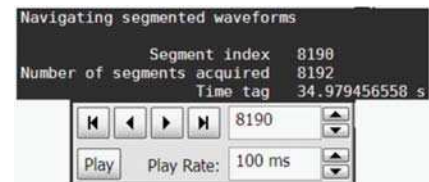

Long time captures using segmented memory


In this example, MIPI DigRF v4 traffic was captured for near 35 seconds. Segmented memory uses time tags to track time between segment acquisitions.

# MIPI DigRF v4 (M-PHY) protocol decode




## Time correlation with other system activity

Protocol measurements are automatically time-correlated with measurements taken on other analog or digital (on MSO models) channels.

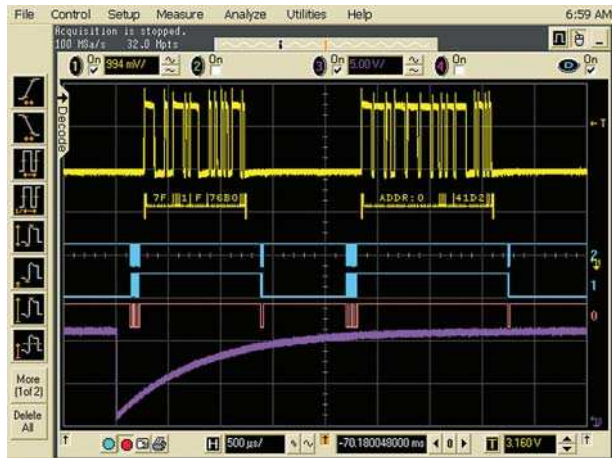

## Precise MSO triggering and display

Mixed-signal oscilloscope measurement in a mobile system using both digital and analog acquisition channels.

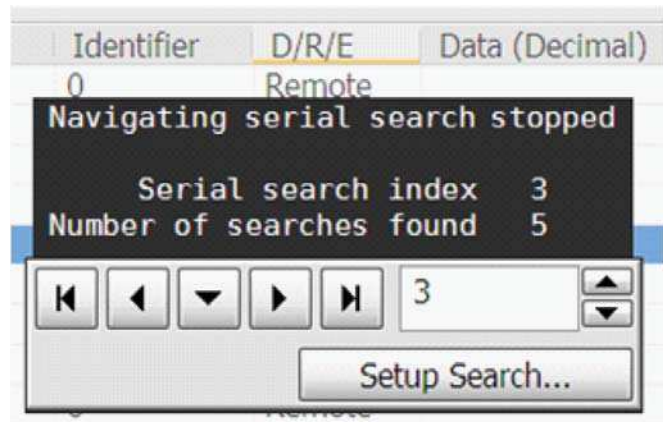

## Post-acquisition searching

Search acquired protocol listings using a menu that is identical to the trigger menu. Quickly move to next occurrence of a specified event.

## MIPI DigRF v4 (M-PHY) application specifications and characteristics

| MIPI                        |  |
|-----------------------------|--|
| MIPI sources                | Analog channels 1, 2, 3, or 4<br>Any waveform memories<br>The application relies on probing and trigger/measurement thresholds to properly condition the signal for triggering and decode. Differential probing may be required. |
| Data rate                   | Up to 6 Gbps   |
| Protocol type               | DigRF v4 v1.00.00  |
| Auto setup                  | Automatically configures scope settings for proper MIPI DigRF v4 decode and SW-based protocol search including memory depth, edge triggering, holdoff, sample rate, and measurement thresholds                                   |
| Decoded fields              | All including extended frame format  |
| Triggering (software-based) | DLC frame<br>SDLC frame<br>Tx frames<br>Rx frames<br>Symbol sequence<br>Error  |

## Ordering Information

### Ordering Information

This application is compatible with all 9000 and 90000, 90000 X-Series oscilloscope models with version 3.50 or greater software.

| Software applications                        | Factory-installed option for new 90000 Series scopes | User-installed stand-alone product number | Server-based license (N5435A option) |
|--|--|---|--------------------------------------|
| MIPI DigRF v4 protocol triggering and decode | 051  | N8807A                                    | 047                                  |

To purchase the protocol triggering and decode features on existing Agilent Infiniium Series oscilloscopes, order the model number shown:

| Model Number  | Description  | Quantity |
|---|--|----------|
| DSO/DSAX91604A<br>or<br>DSO/DSA90604A<br>or<br>DSO/MS09404A | Infiniium Series oscilloscope  | 1        |
| 1132A   | InfiniiMax 5-GHz differential probe amplifier (quantity 3 is recommended for low-speed [SYS-BURST] decode) | 2        |
| E2669A  | Differential probe connectivity kit (contains needed probe heads)  | 1        |

## Related Literature

| Publication title   | Publication type | Publication number |
|---|------------------|--------------------|
| <i>Infiniium 9000 Series Oscilloscopes</i>                                    | Data Sheet       | 5990-3746EN        |
| <i>Infiniium 90000 X-Series Oscilloscopes</i>                                 | Data Sheet       | 5990-5271EN        |
| <i>Infiniium 90000 Series Oscilloscopes</i>                                   | Data Sheet       | 5989-7819EN        |
| <i>U7238A MIPI D-PHY Compliance Test Software for Infiniium oscilloscopes</i> | Data Sheet       | 5990-9337EN        |



## Agilent Technologies Oscilloscopes

Multiple form factors from 20 MHz to >90 GHz | Industry leading specs | Powerful applications



### Agilent Email Updates

[www.agilent.com/find/emailupdates](http://www.agilent.com/find/emailupdates)

Get the latest information on the products and applications you select.



[www.axistandard.org](http://www.axistandard.org)

AdvancedTCA<sup>®</sup> Extensions for Instrumentation and Test (AXIe) is an open standard that extends the AdvancedTCA for general purpose and semiconductor test. Agilent is a founding member of the AXIe consortium.



[www.lxistandard.org](http://www.lxistandard.org)

LAN eXTensions for Instruments puts the power of Ethernet and the Web inside your test systems. Agilent is a founding member of the LXI consortium.



[www.pxisa.org](http://www.pxisa.org)

PCI eXTensions for Instrumentation (PXI) modular instrumentation delivers a rugged, PC-based high-performance measurement and automation system.

### Agilent Channel Partners

[www.agilent.com/find/channelpartners](http://www.agilent.com/find/channelpartners)

Get the best of both worlds: Agilent's measurement expertise and product breadth, combined with channel partner convenience.

Windows<sup>®</sup> is a U.S. registered trademark of Microsoft Corporation.



Agilent Advantage Services is committed to your success throughout your equipment's lifetime. We share measurement and service expertise to help you create the products that change our world. To keep you competitive, we continually invest in tools and processes that speed up calibration and repair, reduce your cost of ownership, and move us ahead of your development curve.

[www.agilent.com/find/advantageservices](http://www.agilent.com/find/advantageservices)



[www.agilent.com/quality](http://www.agilent.com/quality)

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at:

[www.agilent.com/find/contactus](http://www.agilent.com/find/contactus)

#### Americas

|               |                |
|---------------|----------------|
| Canada        | (877) 894 4414 |
| Brazil        | (11) 4197 3600 |
| Mexico        | 01800 5064 800 |
| United States | (800) 829 4444 |

#### Asia Pacific

|                    |                |
|--------------------|----------------|
| Australia          | 1 800 629 485  |
| China              | 800 810 0189   |
| Hong Kong          | 800 938 693    |
| India              | 1 800 112 929  |
| Japan              | 0120 (421) 345 |
| Korea              | 080 769 0800   |
| Malaysia           | 1 800 888 848  |
| Singapore          | 1 800 375 8100 |
| Taiwan             | 0800 047 866   |
| Other AP Countries | (65) 375 8100  |

#### Europe & Middle East

|                |                      |
|----------------|----------------------|
| Belgium        | 32 (0) 2 404 93 40   |
| Denmark        | 45 45 80 12 15       |
| Finland        | 358 (0) 10 855 2100  |
| France         | 0825 010 700*        |
|                | *0.125 €/minute      |
| Germany        | 49 (0) 7031 464 6333 |
| Ireland        | 1890 924 204         |
| Israel         | 972-3-9288-504/544   |
| Italy          | 39 02 92 60 8484     |
| Netherlands    | 31 (0) 20 547 2111   |
| Spain          | 34 (91) 631 3300     |
| Sweden         | 0200-88 22 55        |
| United Kingdom | 44 (0) 118 927 6201  |

For other unlisted countries:

[www.agilent.com/find/contactus](http://www.agilent.com/find/contactus)

Revised: January 6, 2012

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 2012  
Published in USA, July 20, 2012  
5990-9020EN

