

# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

# 090AAS



### Highlights & Features

- Compliant to IEC 60601-1 3rd edition
- IT and medical safety approvals
- Low earth leakage current (<0.1mA)
- Overload, over voltage, over temperature and short circuit protections
- Risk management report available
- Energy Star Compliance (Level V)\
- 2 x MOPP(means of patient protection)

### Safety Standards



CB Certified for worldwide use

**Model Number:** MDS-090AAS19 BA  
**Unit Weight:** 0.45kg  
**Dimensions (W x L x H):** 60.0x150.0x35.0 mm  
 2.4x5.9x1.4 in

### General Description

The MDS series of external power supply comes with universal AC input at 90Vac to 264Vac. Other features include low earth leakage, risk management report available and the electric shock protection comply with 2 x MOPP. The MDS series is certified for EMC standards according to EN 55011 for industrial, scientific and medical (ISM) radio-frequency equipment and EN 55022 for Industrial Technology Equipment (ITE) radio-frequency equipment. In addition, only recognized Japanese capacitors are used.

The MDS series come with both medical and ITE safety approvals including UL/CSA/CCC/CE and CB certification and are fully compliant with RoHS Directive 2011/65/EU for environmental protection.

### Model Information

Medical AC-DC Adapter

| Model Number    | Input Voltage Range | Output Voltage | Output Current |
|-----------------|---------------------|----------------|----------------|
| MDS-090AAS19 BA | 90-264Vac           | 19Vdc          | 4.73A          |

### Model Numbering

| MDS                        | 090  | A                   | A                          | S   | 19  | B   | A   |
|----------------------------|--|---------------------|----------------------------|---|---|---|---|
| Delta Medical power Supply | Max wattage in the product Series. Maybe lower at some voltage.<br>060 → 60W<br>120 → 120W<br>1K2 → 1,200W | Family Code<br>A~ Z | Product Type<br>A: Adapter | Output Code<br>S: Single Output<br>2: Dual Output<br>3: Triple Output<br>4: Four Output<br>5: More than Five Output | Output Voltage<br>Single Output:<br>- 03 for 3.3V<br>- 05 for 5V<br>- 12 for 12V<br>Multiple Output:<br>Serial Number<br>00 to 99 | Input Connector code<br>B: Socket C14 / 3 Pin<br>D: Socket C6 / 3 Pin | Output Connector code<br>A: 4 pin DIN/1200mm<br>B: 4 pin DIN/1800mm<br>E = barrel type 5.5*2.5, L=10mm/1200mm<br>F = barrel type 5.5*2.5, L=10mm/1800mm<br>J = barrel type 5.5*1.7, L=10mm/1200mm<br>K = barrel type 5.5*1.7, L=10mm/1800mm |



# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Specifications

#### Input Ratings / Characteristics

|                             |  |
|-----------------------------|--|
| Nominal Input Voltage       | 100-240Vac   |
| Input Voltage Range         | 90-264Vac  |
| Nominal Input Frequency     | 50-60Hz  |
| Input Frequency Range       | 47-63Hz  |
| Input Current (max)         | 2A @ 115Vac, 1A @ 230Vac   |
| Efficiency (typ.)           | 91.7%, Ref. Reference Fig.1  |
| Standby Power (max)         | 0.5W   |
| Inrush Current (typ.)       | 50A @ 115Vac, 100A @ 230Vac  |
| Earth Leakage Current (max) | 0.1mA @ 264Vac NC <sup>1)</sup> , 0.3mA @ 264Vac SFC <sup>2)</sup> |

1) NC: normal condition

2) SFC: single fault condition

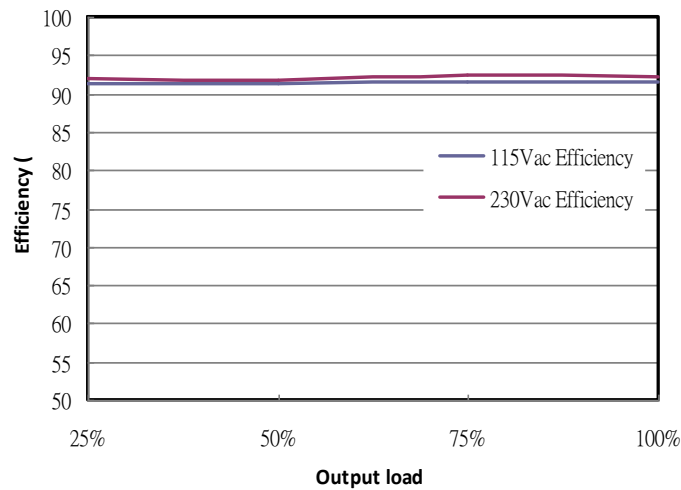


Fig.1 Efficiency versus output load

#### Output Ratings / Characteristics

|   |   |
|---|---|
| Nominal Output Voltage                                | 15Vdc                                     |
| Output Voltage Tolerance                              | ± 5%                                      |
| Output Current  | 4.73A                                     |
| Output Power  | 90W                                       |
| Line Regulation (max)                                 | ±0.5%                                     |
| Load Regulation (max)                                 | ±5%                                       |
| Ripple & Noise (typ.)                                 | 91mV pk-pk @ Full load, Reference Fig. 2, |
| Start-up Time (max)                                   | 3000ms                                    |
| Hold-up Time (min)                                    | 20ms @ 115Vac&230Vac                      |
| Dynamic Response (Overshoot & Undershoot O/P Voltage) | ± 5% @ 50-100% load                       |

# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA


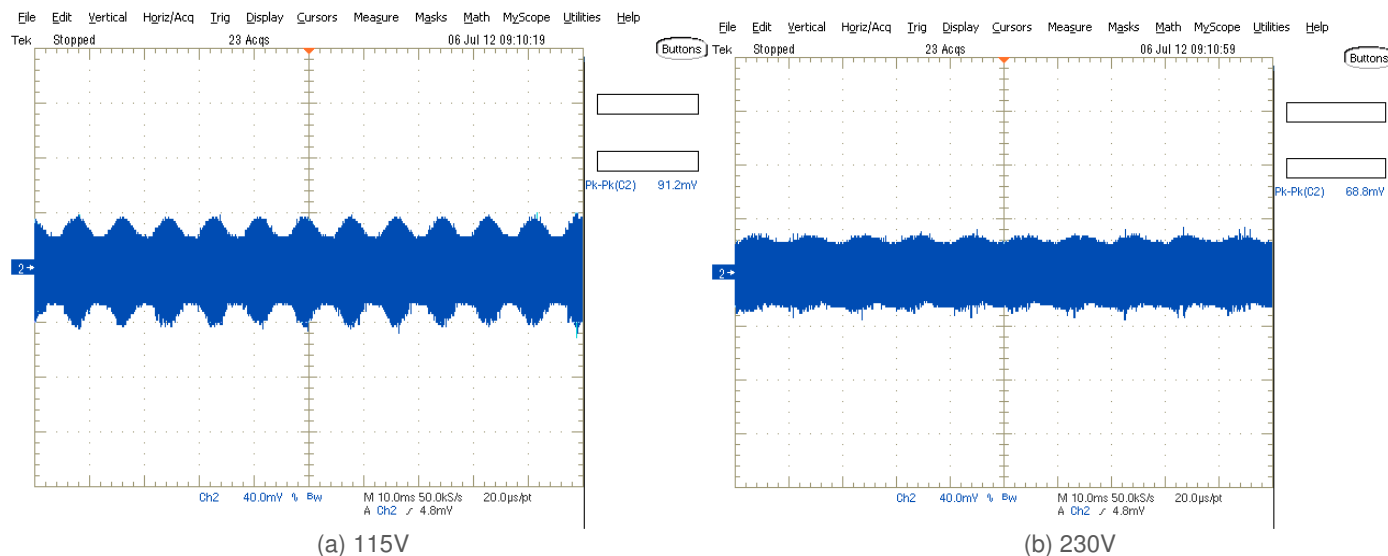


Fig. 2 Ripple & Noise example, 20MHz BW

Ripple & Noise measurement circuit

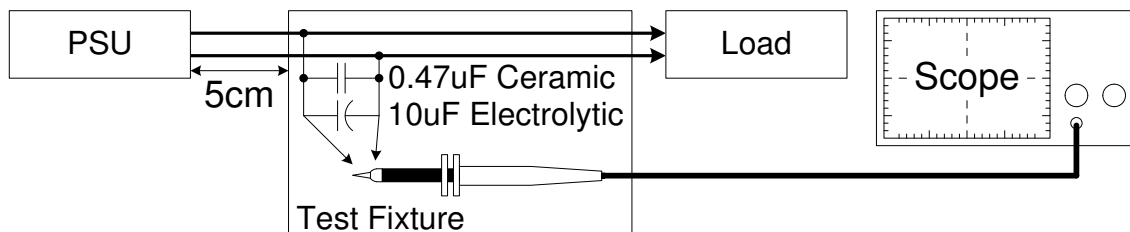

### Mechanical

|                      |                                       |
|----------------------|---------------------------------------|
| Case Chassis         | PC                                    |
| Case Cover           | PC                                    |
| Dimensions(W x Lx H) | 60.0x 150.0 x 35.0 mm(2.4x5.9x1.4 in) |
| Unit Weight          | 0.45kg                                |
| Indicator            | NA                                    |
| Cooling System       | NA                                    |
| Terminal             | Input C14 socket                      |
|                      | Output 4 Pin Din                      |

### Environment

|                             |           |  |
|-----------------------------|-----------|--|
| Surrounding Air Temperature | Operating | 0°C to +40 °C                                    |
|                             | Storage   | -40 °C to +85 °C                                 |
| Operating Humidity          |           | 10-95% RH (Non-Condensing)                       |
| Operating Altitude          |           | 3,000 meters                                     |
| Shock Test (Non-Operating)  |           | 50G, 11ms, 3 shocks for each direction           |
| Vibration (Operating)       |           | 5-500Hz, 2.09Grms, 20 minute for each three axis |

# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Protections

|                                 |  |
|---------------------------------|--|
| Overvoltage (max.)              | 150%, Latch Mode   |
| Over load / Over current (max.) | 130% of rated load current, Hiccup Mode, (Non-Latching, Auto-Recovery) |
| Over Temperature                | Hiccup Mode, (Non-Latching, Auto-Recovery)                             |
| Short Circuit                   | Hiccup Mode, (Non-Latching, Auto-Recovery)                             |
| Degree of Protection            | IP40   |
| Protection Against Shock        | Class II with functional earth   |

### Reliability Data

|             |                                      |
|-------------|--------------------------------------|
| MTBF (typ.) | 1139 kHrs based on Telecordia SR-332 |
|-------------|--------------------------------------|

### Safety Standards / Directives

|                    |  |
|--------------------|--|
| Medical Safety     | IEC60601-1: (Ed.3,2005), EN0601-1:2006, CAN/CSA-C22.2 No. 60601-1:08, ANSI/AAMI ES60601-1: (Ed.3,2005) |
| ITE Safety         | IEC60950-1 (Ed.2,2005), GB4943.1-2011, GB9254-2008, GB17625.1-2003                                     |
| CE                 | MDD Directive 93/42/EEC  |
| Material and Parts | RoHS Directive 2011/65/EU Compliant  |
| Galvanic Isolation | Input to Output<br>4000 Vac  |

# MDS Medical AC-DC Adapter


## 19V 90W / MDS-090AAS19 BA

### EMC

|                                   |   |  |
|-----------------------------------|---|--|
| EMC / Emissions                   | EN55011, EN55022, FCC Title 47: Class B |  |
| Immunity to                       |   |  |
| Voltage Flicker                   | IEC61000-3-3                            |  |
| Electrostatic Discharge           | IEC61000-4-2                            | Level 3 Criteria A <sup>1)</sup><br>Air Discharge: 8kV<br>Contact Discharge: 6kV                             |
| Radiated Field                    | IEC61000-4-3                            | Level 2 Criteria A <sup>1)</sup><br>80MHz-1GHz, 3V/M with 1kHz tone / 80% modulation                         |
| Electrical Fast Transient / Burst | IEC61000-4-4                            | Level 3 Criteria A <sup>1)</sup><br>2kV  |
| Surge                             | IEC61000-4-5                            | Level 3 Criteria A <sup>1)</sup><br>Common Mode <sup>2)</sup> : 2kV<br>Differential Mode <sup>3)</sup> : 1kV |
| Conducted                         | IEC61000-4-6                            | Level 2 Criteria A <sup>1)</sup><br>150kHz-80MHz, 3Vrms  |
| Power Frequency Magnetic Fields   | IEC61000-4-8                            | Criteria A <sup>1)</sup><br>Magnetic field strength 3A/Meter   |
| Voltage Dips                      | IEC61000-4-11                           | 30% 10ms Criteria A ; 60% 100ms and 100% 5000ms<br>Criteria B  |

1) Criteria A: Normal performance within the specification limits  
 2) Asymmetrical: Common mode (Line to earth)  
 3) Symmetrical: Differential mode (Line to line)

### Block Diagram

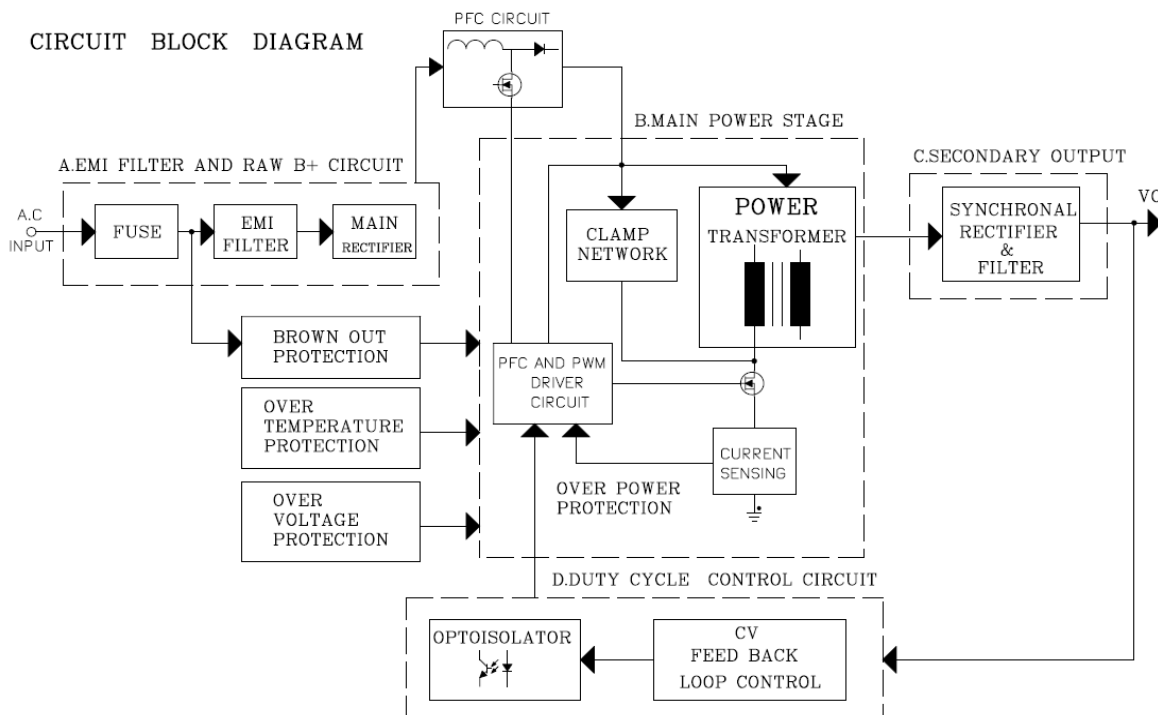


# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Dimensions

L x W x H: 60.0x 150.0 x 35.0 mm

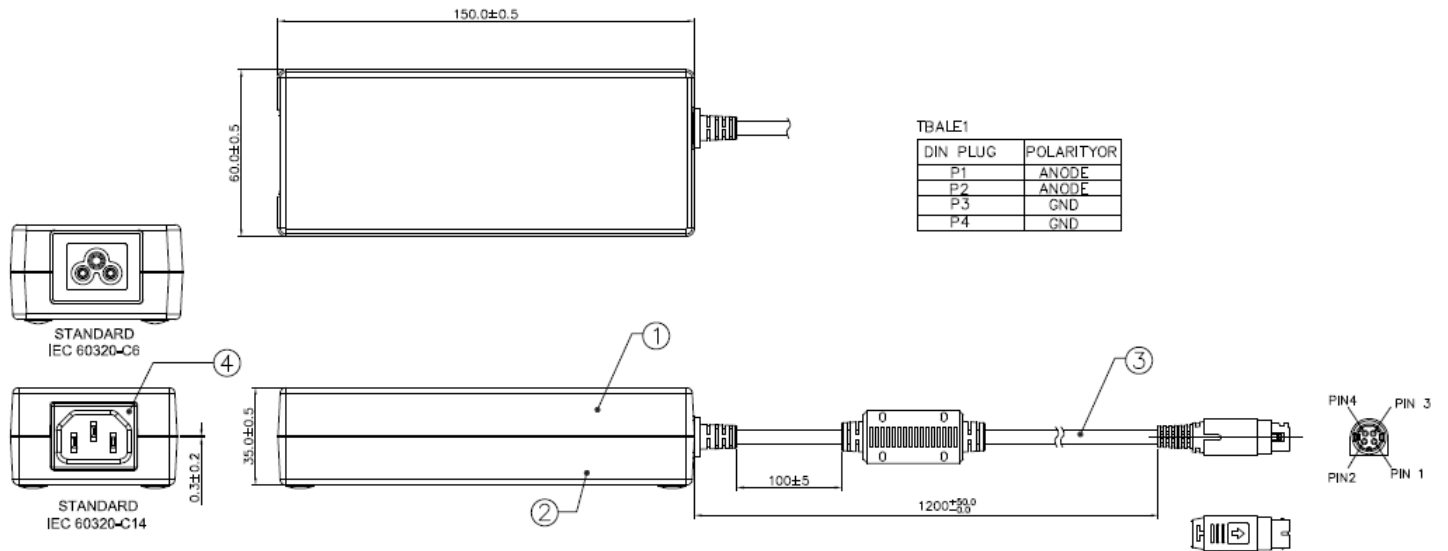

### Notes

- Dimensions are in mm

| Item | Device Description |
|------|--------------------|
| 1    | Cover              |
| 2    | Chassis            |
| 3    | Power Cord         |
| 4    | Socket             |

# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Functions

#### Start-up Time

The time required for the output voltage to reach 90% of its set value, after the input voltage is applied.


#### Rise Time

The time required for the output voltage to change from 10% to 90% of its set value.

#### Hold-up Time

Hold up time is the time when the AC input collapses and output voltage retains regulation for a certain period of time. The time required for the output to reach 95% of its set value, after the input voltage is removed.

### ■ Graph illustrating the Start-up Time, Rise Time, and Hold-up Time

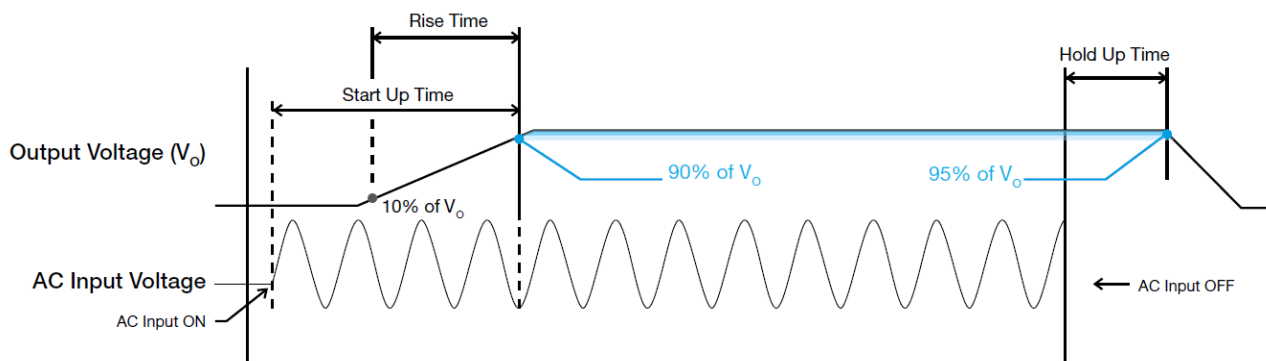


# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Dynamic Response


The power supply output voltage will remain within  $\pm 5\%$  of its steady state value, when subjected to a dynamic load 50 to 100% of its rated current.

■ 50 to 100% Load

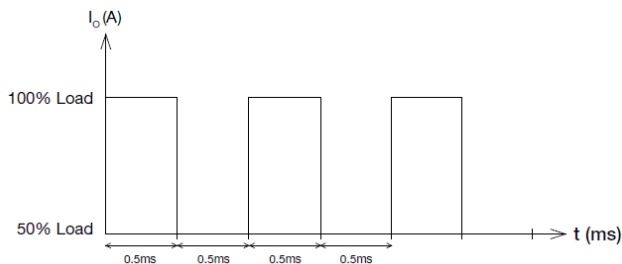

### Inrush Current

Inrush current is the peak, instantaneous, input current measured and, occurs when the input voltage is first applied. For AC input voltages, the maximum peak value of inrush current will occur during the first half cycle of the applied AC voltage. This peak value decreases exponentially during subsequent cycles of AC voltage.

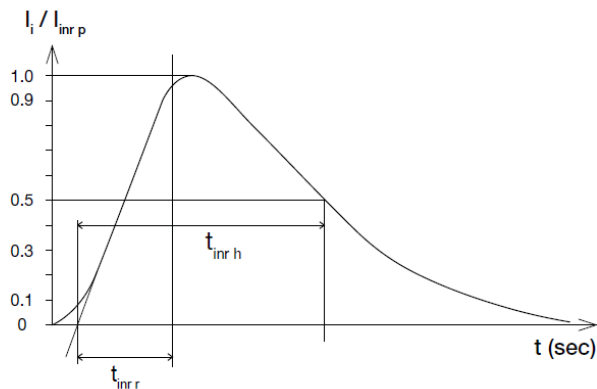

### Overvoltage Protection


The power supply's overvoltage circuit will be activated when its internal feedback circuit fails. The output voltage shall not exceed its specifications defined on Page 3 under "Protections". Power supply will latch off, and require removal/re-application of input AC voltage in order to restart.

### Short Circuit Protection

The power supply's output OLP/OCP function also provides protection against short circuits. When a short circuit is applied, the output current will operate in "Hiccup mode", as shown in the illustration in the OLP/OCP section on this page. The power supply will return to normal operation after the short circuit is removed.

### Overload & Over current Protections

The power supply's Overload (OLP) and Over current (OCP) Protections will be activated when output current under 130% of  $I_O$  (Max load). In such occurrence, the  $V_O$  will start to droop and once the power supply has reached its maximum power limit, the protection is activated and the power supply will go into "Hiccup mode" (Auto-Recovery). The power supply will recover once the fault condition of the OLP and OCP is removed and  $I_O$  is back within the specifications.

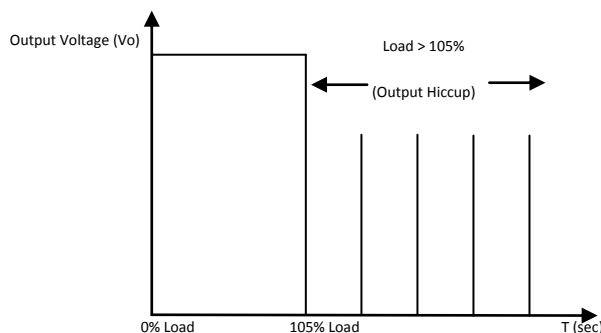

Additionally, if the  $I_O$  is  $< 105\%$  but  $> 100\%$  for a prolonged period of time (depending on the load), the Over Temperature Protection (OTP) will be activated due to high temperature on critical components. The power supply will then go into hiccup mode until the fault is removed and the mains is reapplied.

### Over Temperature Protection

As mentioned above, the power supply also has Over Temperature Protection (OTP). This is activated when the overload condition persists for an extended duration and the output current is below the overload trigger point but  $> 100\%$  load. In the event of a higher operating condition at 100% load, the power supply will run into OTP when the surrounding air temperature is higher than the operating temperature. When activated, the output voltage will go into latch mode until the main is reapplied and the surrounding air temperature drops to its normal operating temperature.

# MDS Medical AC-DC Adapter

## 19V 90W / MDS-090AAS19 BA

### Certificate



All Delta Medical Power products conform to the European directive 2011/65/EU. RoHS is the abbreviation for "Restriction of the use of certain hazardous substances".



Delta has been certified as meeting the requirement of ISO 13485: 2003 and EN ISO 13485: 2012 for the design and manufacture of switching power supply and adaptor for medical device.



In addition to an UL Total Certification Program (TCP) approved client laboratory for IEC 62368-1. Delta also has participated UL Client Test Data Program (CTDP) for IEC 60601.



Energy star level V compliance